Chandra X-ray Center

Instrument: HRC
Source: VEGA
Title: TEST OF UV SENSITVITY

Seq Num: 290088
Obs ID: 1806
PI: Dr. CXC Calibration

hrcf01806N005 full img2.fits	hrcf01806N005 cntr img2.fits

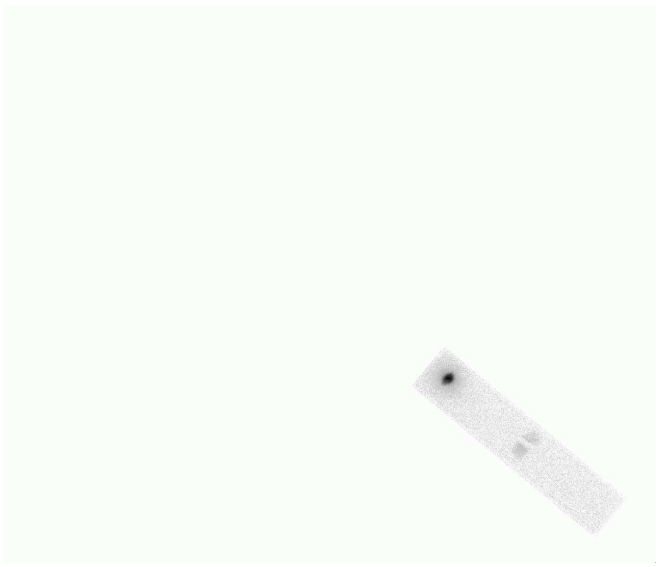

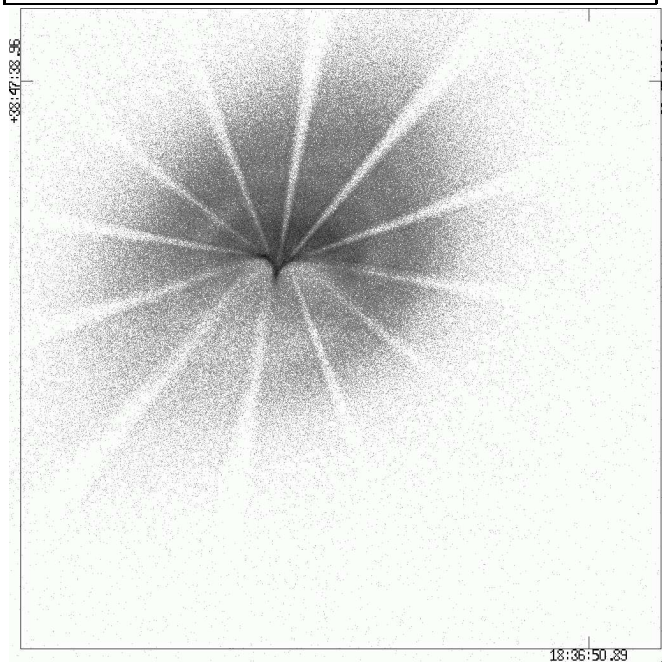

Chandra X-ray Center
Seq Num: 290088
Instrument: HRC
Obs ID: 1806
Source: VEGA
PI: Dr. CXC Calibration
Title: TEST OF UV SENSITVITY

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.10	Processing system revision
DATE	2007-06-02T04:09:28	Date and time of file creation
DATE-OBS	2000-08-06T11:21:11	Observation start date
DATE-END	2000-08-06T12:19:41	Observation end date
RA_PNT	279.55549896285	Pointing RA
DEC_PNT	38.989379745834	Pointing Dec
ROLL_PNT	219.61337660974	Pointing Roll
RA_TARG	279.230833	Observer's specified target RA
DEC_TARG	38.7795	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.10	Processing system revision
DATE	2007-06-02T04:32:12	Date and time of file creation
DATE-OBS	2000-08-06T11:21:11	Observation start date
DATE-END	2000-08-06T12:19:41	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	NONE	Grating
OBJECT	VEGA	Source name
TITLE	TEST OF UV SENSITVITY	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	1806	Observation id
SEQ_NUM	290088	Sequence number
RA_NOM	279.55549896285	Nominal RA
DEC_NOM	38.989379745834	Nominal Dec
ROLL_NOM	219.61337660974	Nominal Roll

Chandra X-ray Center
Seq Num: 290088
Instrument: HRC
Obs ID: 1806
Source: VEGA
PI: Dr. CXC Calibration
Title: TEST OF UV SENSITVITY

Full Field with Sources

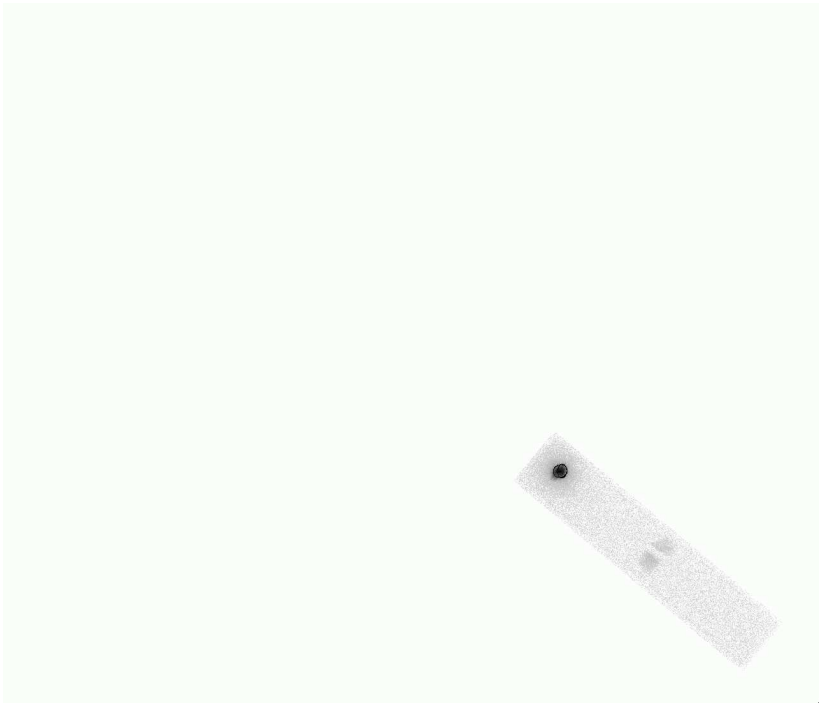

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
279.233089	38.785653	447323.968750	723.468933	618.304321
279.228764	38.785874	84911.007812	685.603638	123.848534