Chandra X-ray Center

Seq Num: 590193

Instrument: HRC

Obs ID: 1744

Source: PSR B0540-69

PI: DR. CXC CALIBRATION

Title: VERIFICATION OF AXAF TIMING CAPABILITY

---

hrcf01744N006 full img2.fits	hrcf01744N006 cntr img2.fits
	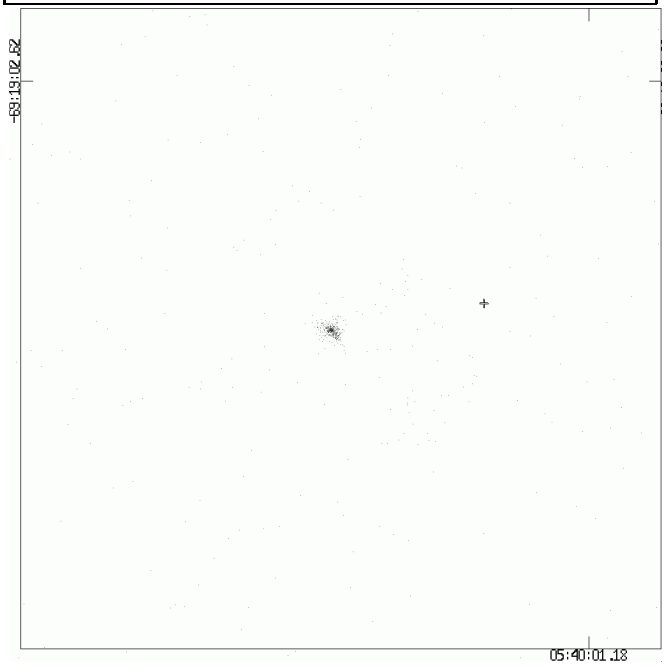

Chandra X-ray Center
Seq Num: 590193
Instrument: HRC
Obs ID: 1744
Source: PSR B0540-69
PI: DR. CXC CALIBRATION
Title: VERIFICATION OF AXAF TIMING CAPABILITY

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.10	Processing system revision
DATE	2007-05-27T08:25:56	Date and time of file creation
DATE-OBS	2000-06-22T14:15:38	Observation start date
DATE-END	2000-06-22T14:23:57	Observation end date
RA_PNT	85.021897006265	Pointing RA
DEC_PNT	-69.330167584436	Pointing Dec
ROLL_PNT	174.02562979227	Pointing Roll
RA_TARG	85.04625	Observer's specified target RA
DEC_TARG	-69.332	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.10	Processing system revision
DATE	2007-05-27T08:43:39	Date and time of file creation
DATE-OBS	2000-06-22T14:15:38	Observation start date
DATE-END	2000-06-22T14:23:57	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	NONE	Grating
OBJECT	PSR B0540-69	Source name
TITLE	VERIFICATION OF AXAF TIMING CAPABILITY	Proposal title
OBSERVER	DR. CXC CALIBRATION	Principal investigator
OBS_ID	1744	Observation id
SEQ_NUM	590193	Sequence number
RA_NOM	85.021897006265	Nominal RA
DEC_NOM	-69.330167584436	Nominal Dec
ROLL_NOM	174.02562979227	Nominal Roll

Chandra X-ray Center
Seq Num: 590193
Instrument: HRC
Obs ID: 1744
Source: PSR B0540-69
PI: DR. CXC CALIBRATION
Title: VERIFICATION OF AXAF TIMING CAPABILITY

Full Field with Sources

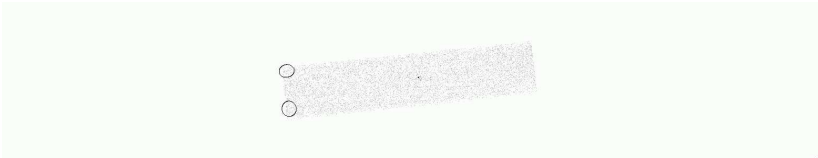

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
85.046753	-69.331663	132.500000	17.568430	7.541937
85.878765	-69.315430	31.387501	9.079083	3.457122
85.866173	-69.398984	33.830357	11.010020	3.072688