Chandra X-ray Center

Seq Num: 590062

Instrument: ACIS

Obs ID: 194

Source: CAS A [Chip I3, T=120, Offsets=-2,2,0]

PI: Dr. CXC Calibration

Title: ACIS CHIP RESPONSE TO CAS A, JUL. 99

---

acisf00194N003 full img2.fits	acisf00194N003 cntr img2.fits

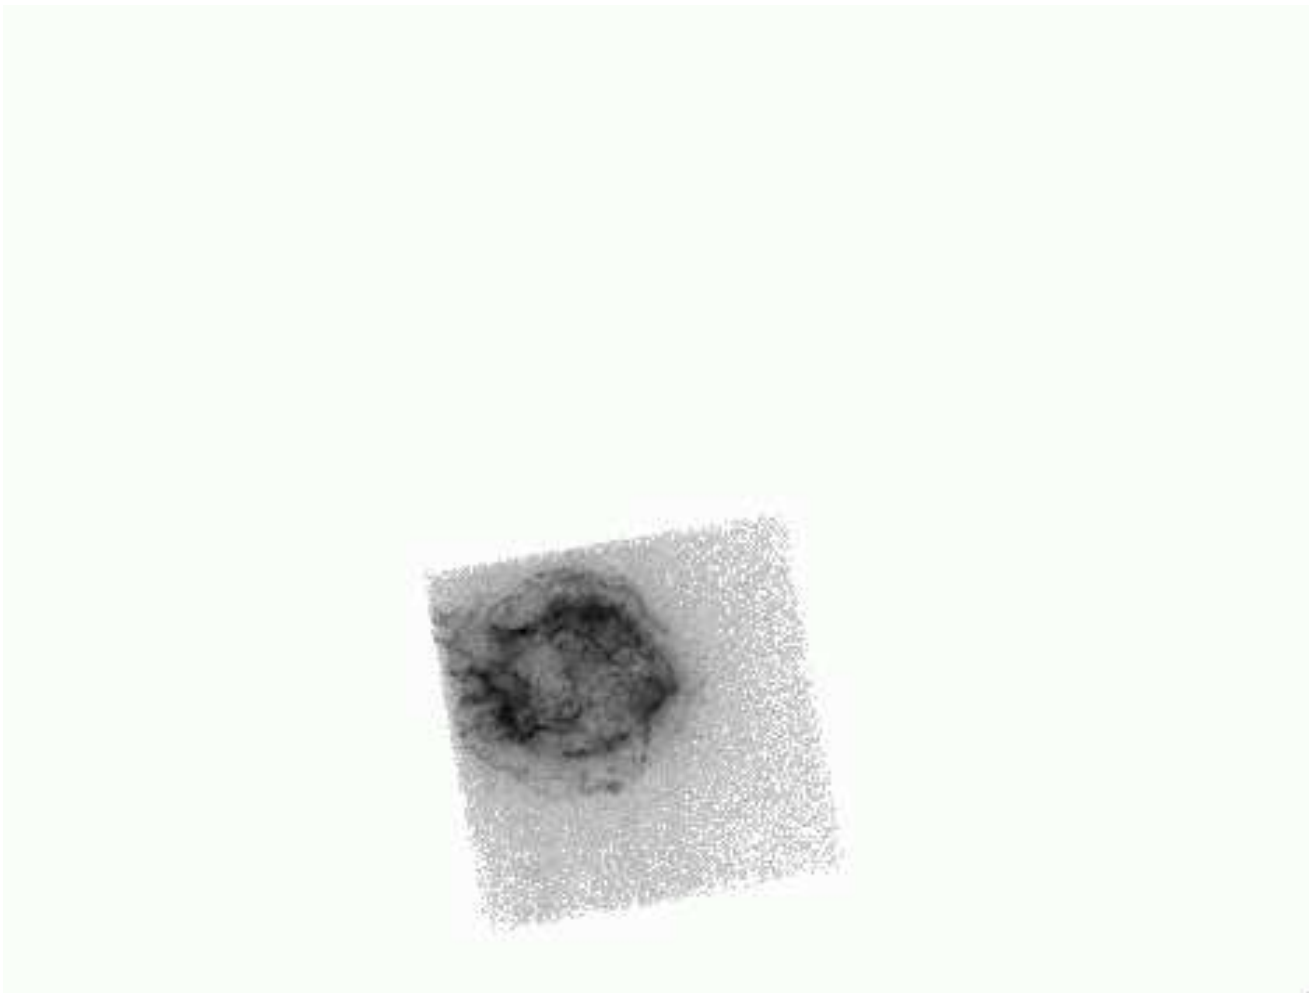

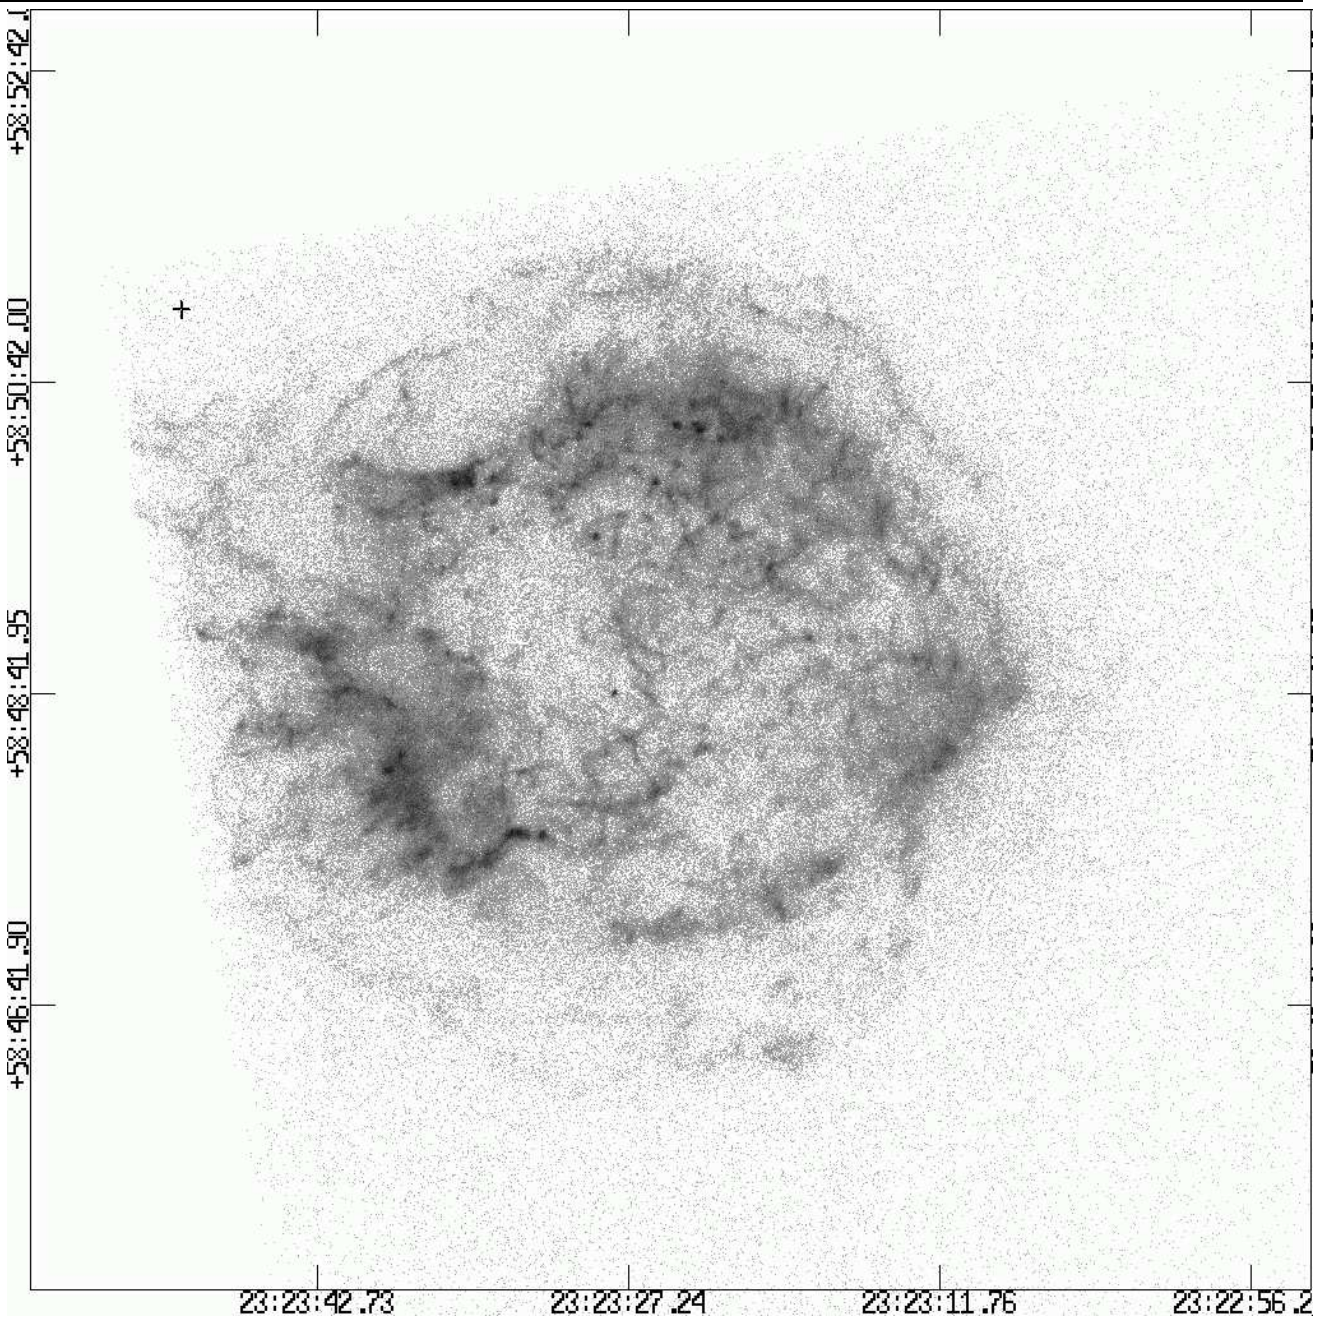

Chandra X-ray Center

Seq Num: 590062

Instrument: ACIS

Obs ID: 194

Source: CAS A [Chip I3, T=120, Offsets=-2,2,0]

PI: Dr. CXC Calibration

Title: ACIS CHIP RESPONSE TO CAS A, JUL. 99

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.10	ASCDS version number
DATE	2007-05-19T10:10:11	Date and time of file creation
DATE-OBS	2000-05-19T17:08:16	Observation start date
DATE-END	2000-05-19T18:59:11	Observation end date
RA_PNT	350.95598101999	Pointing RA
DEC_PNT	58.852757000128	Pointing Dec
ROLL_PNT	80.130372804465	Pointing Roll
RA_TARG	350.8575	Observer's specified target RA
DEC_TARG	58.814833	Observer's specified target Dec
DATAMODE	FAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	153.4460144	Focal Plane Temperature [K]
FSW_VERS	30	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.10	ASCDS version number
DATE	2007-05-19T10:37:05	Date and time of file creation
DATE-OBS	2000-05-19T17:08:16	Observation start date
DATE-END	2000-05-19T18:59:11	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-012367	Detector
GRATING	NONE	Grating
OBJECT	CAS A [Chip I3, T=120, Offsets=-2,2,0]	Source name
TITLE	ACIS CHIP RESPONSE TO CAS A, JUL. 99	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	194	Observation id
SEQ_NUM	590062	Sequence number
RA_NOM	350.95598101999	Nominal RA
DEC_NOM	58.852757000128	Nominal Dec
ROLL_NOM	80.130372804465	Nominal Roll

Chandra X-ray Center

Seq Num: 590062

Instrument: ACIS

Obs ID: 194

Source: CAS A [Chip I3, T=120, Offsets=-2,2,0]

PI: Dr. CXC Calibration

Title: ACIS CHIP RESPONSE TO CAS A, JUL. 99

Full Field with Sources

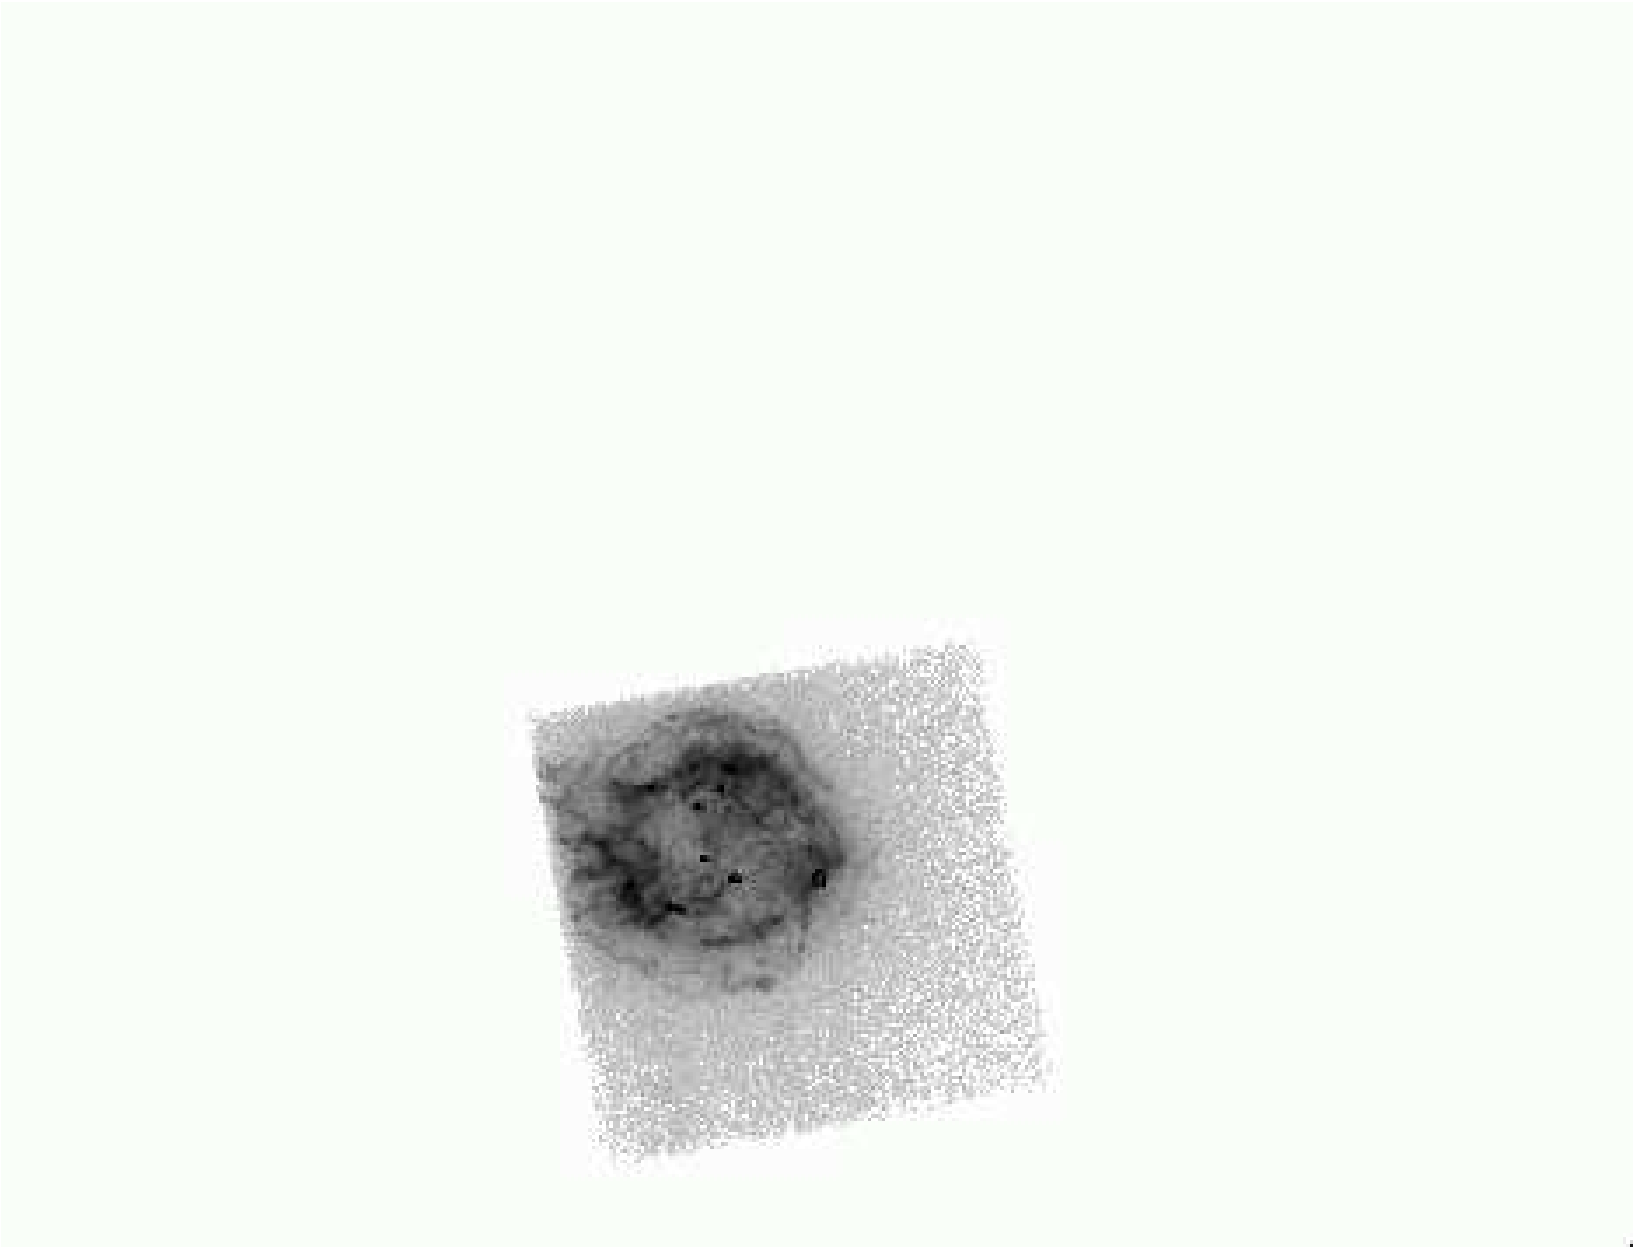

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
350.887369	58.796566	1201.428589	66.495010	18.067951
350.881224	58.796441	832.428589	47.561924	17.501995
350.848873	58.840059	842.477295	53.512409	15.743587
350.853545	58.840433	641.943176	45.540951	14.095954
350.870286	58.828355	439.590912	32.037827	13.720996
350.797750	58.805826	891.965881	65.674461	13.581626
350.866404	58.811716	282.125000	21.772173	12.958054
350.857768	58.834296	437.204559	35.964729	12.156481
350.913085	58.803297	620.238647	51.288513	12.093130
350.848332	58.805711	401.000000	33.179726	12.085694