Chandra X-ray Center

Seq Num: 290141
Obs ID: 2585
PI: Dr. CXC Calibration

Instrument: HRC
Source: HZ43
Grating: LETG
Title: AO3 CALIBRATION OBSERVATIONS OF HZ43

---

hrcf02585N002 full img2.fits	hrcf02585N002 cntr img2.fits
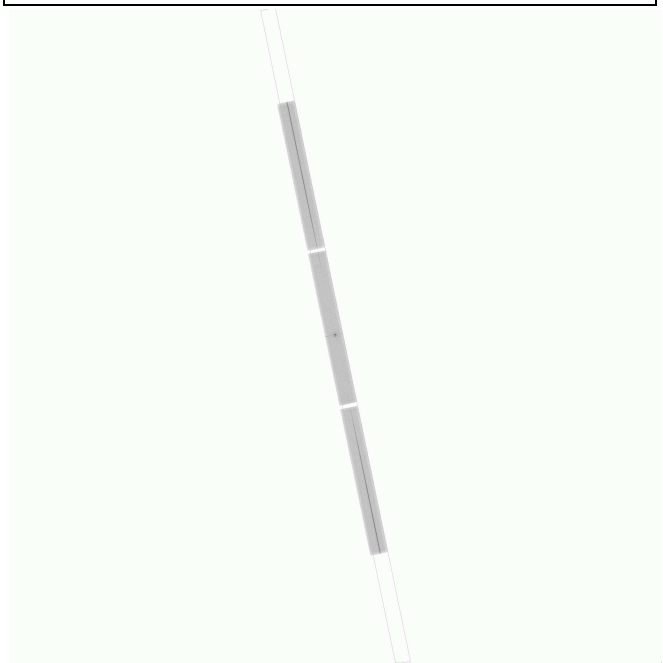	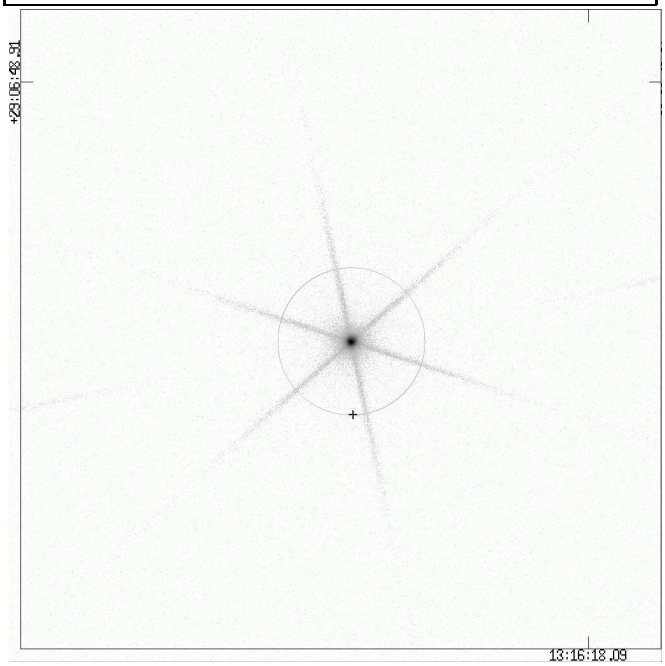

Chandra X-ray Center
Seq Num: 290141
Instrument: HRC
Obs ID: 2585
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO3 CALIBRATION OBSERVATIONS OF HZ43

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.9	ASCDS version number
DATE	2006-09-26T12:24:04	Date and time of file creation
DATE-OBS	2002-07-23T14:01:38	Observation start date
DATE-END	2002-07-23T19:58:54	Observation end date
RA_PNT	199.09081144751	Pointing RA
DEC_PNT	29.094480721695	Pointing Dec
ROLL_PNT	258.23305731771	Pointing Roll
RA_TARG	199.092083	Observer's specified target RA
DEC_TARG	29.099	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.9	ASCDS version number
DATE	2006-09-26T12:50:27	Date and time of file creation
DATE-OBS	2002-07-23T14:01:38	Observation start date
DATE-END	2002-07-23T19:58:54	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	LETG	Grating
OBJECT	HZ43	Source name
TITLE	AO3 CALIBRATION OBSERVATIONS OF HZ43	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	2585	Observation id
SEQ_NUM	290141	Sequence number
RA_NOM	199.09081144751	Nominal RA
DEC_NOM	29.094480721695	Nominal Dec
ROLL_NOM	258.23305731771	Nominal Roll

Chandra X-ray Center
Seq Num: 290141
Instrument: HRC
Obs ID: 2585
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO3 CALIBRATION OBSERVATIONS OF HZ43
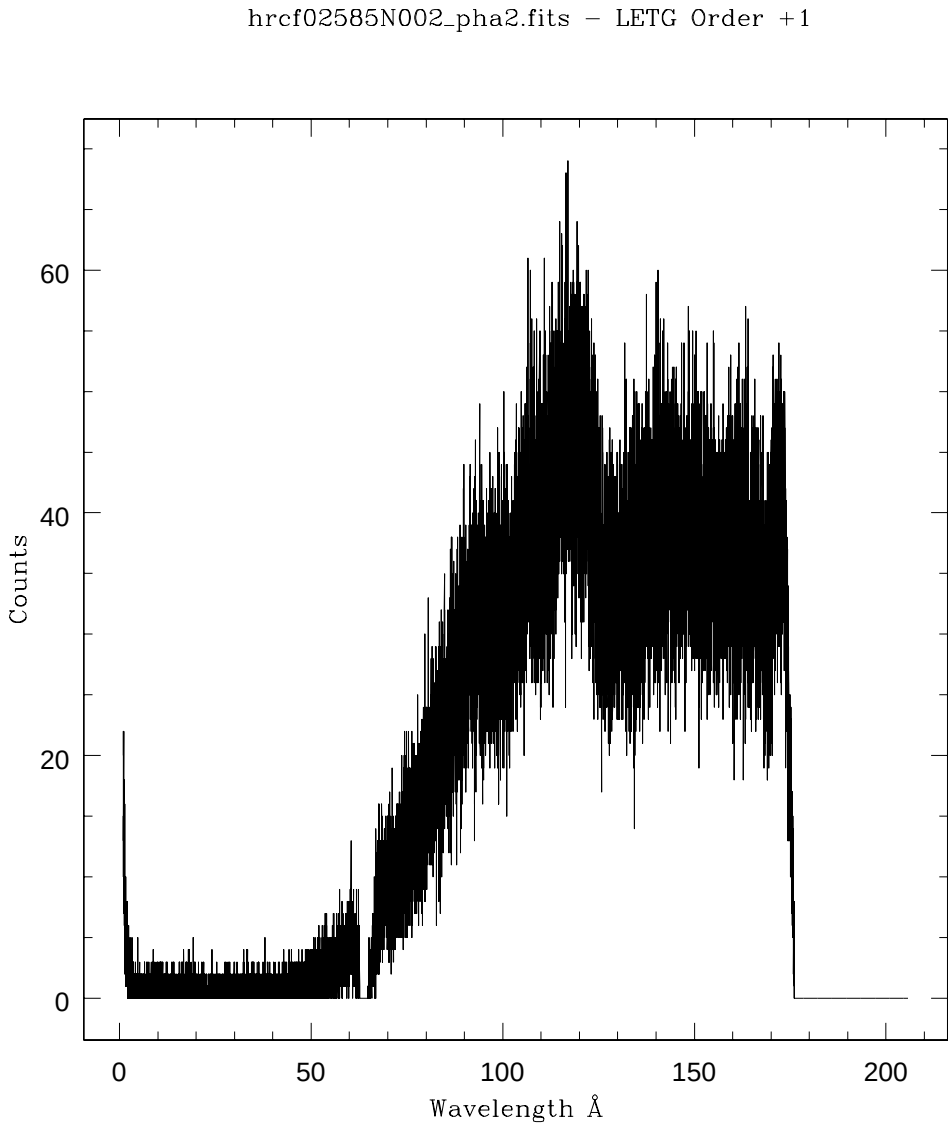
LETG +1 order