Chandra X-ray Center

Seq Num: 590267

Instrument: HRC

Obs ID: 2878

Source: CAS A [HRC-I, Offsets=0,0,0]

PI: Dr. CXC Calibration

Title: AO3B CALIBRATION OBSERVATIONS THE STANDARD CANDLES CAS A AND G21.5-09

---

hrcf02878N003 full img2.fits

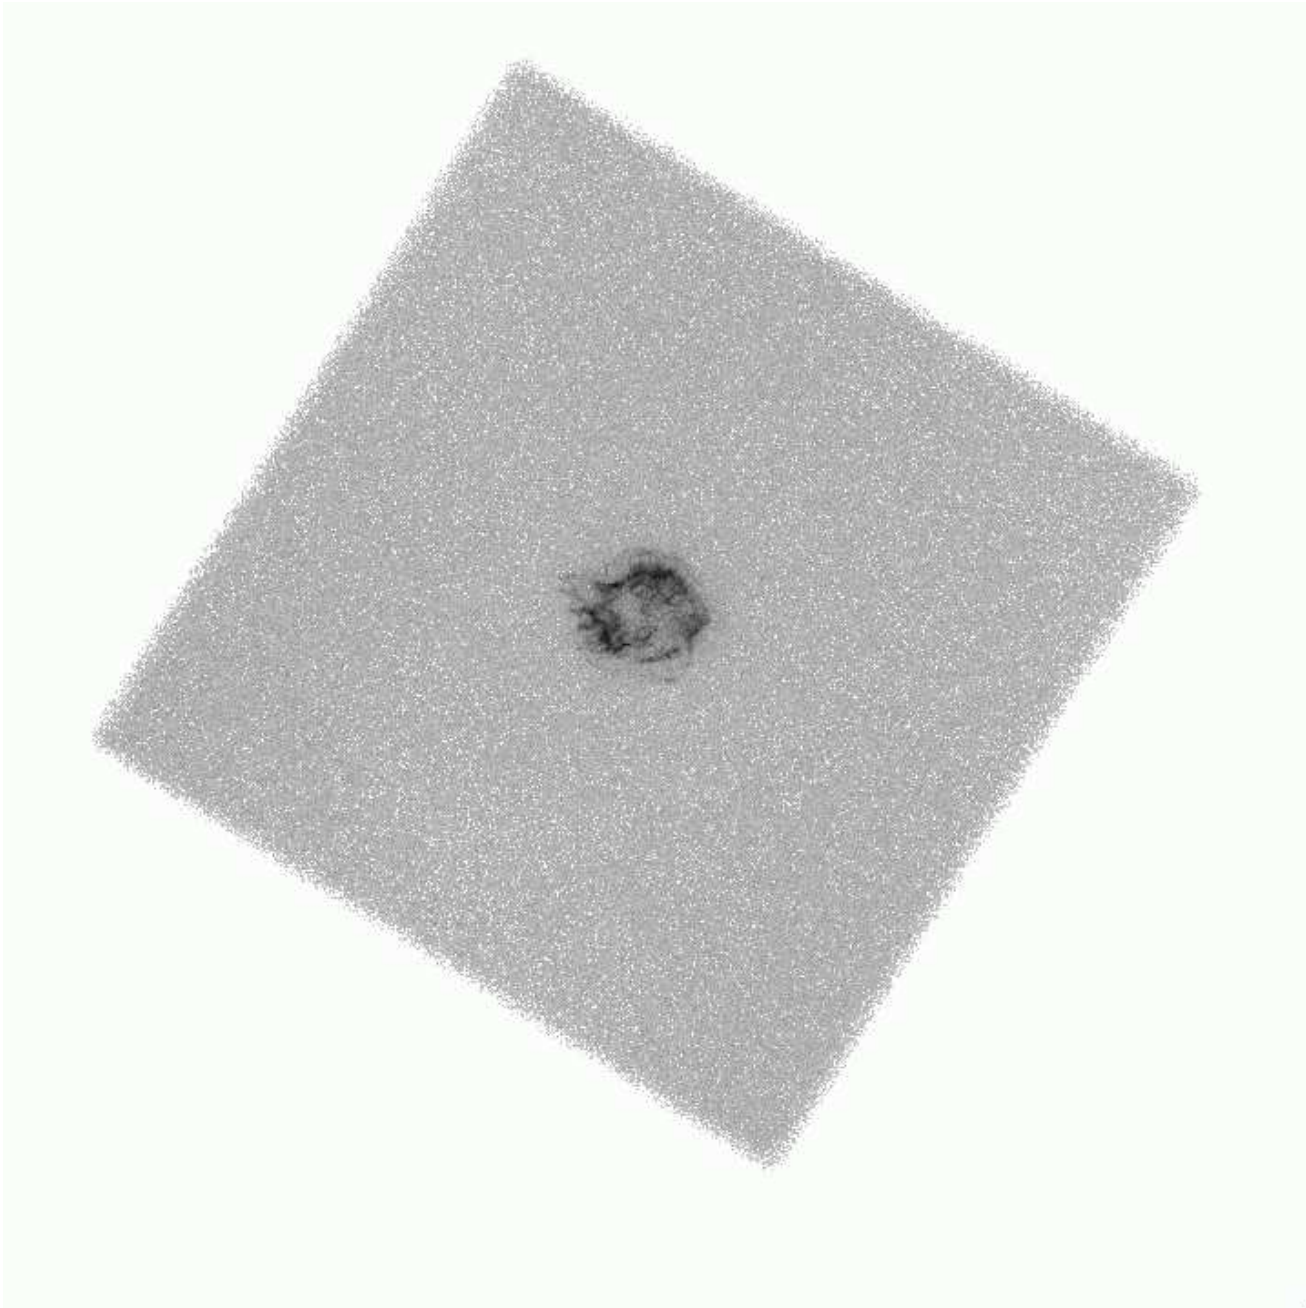

hrcf02878N003 cntr img2.fits

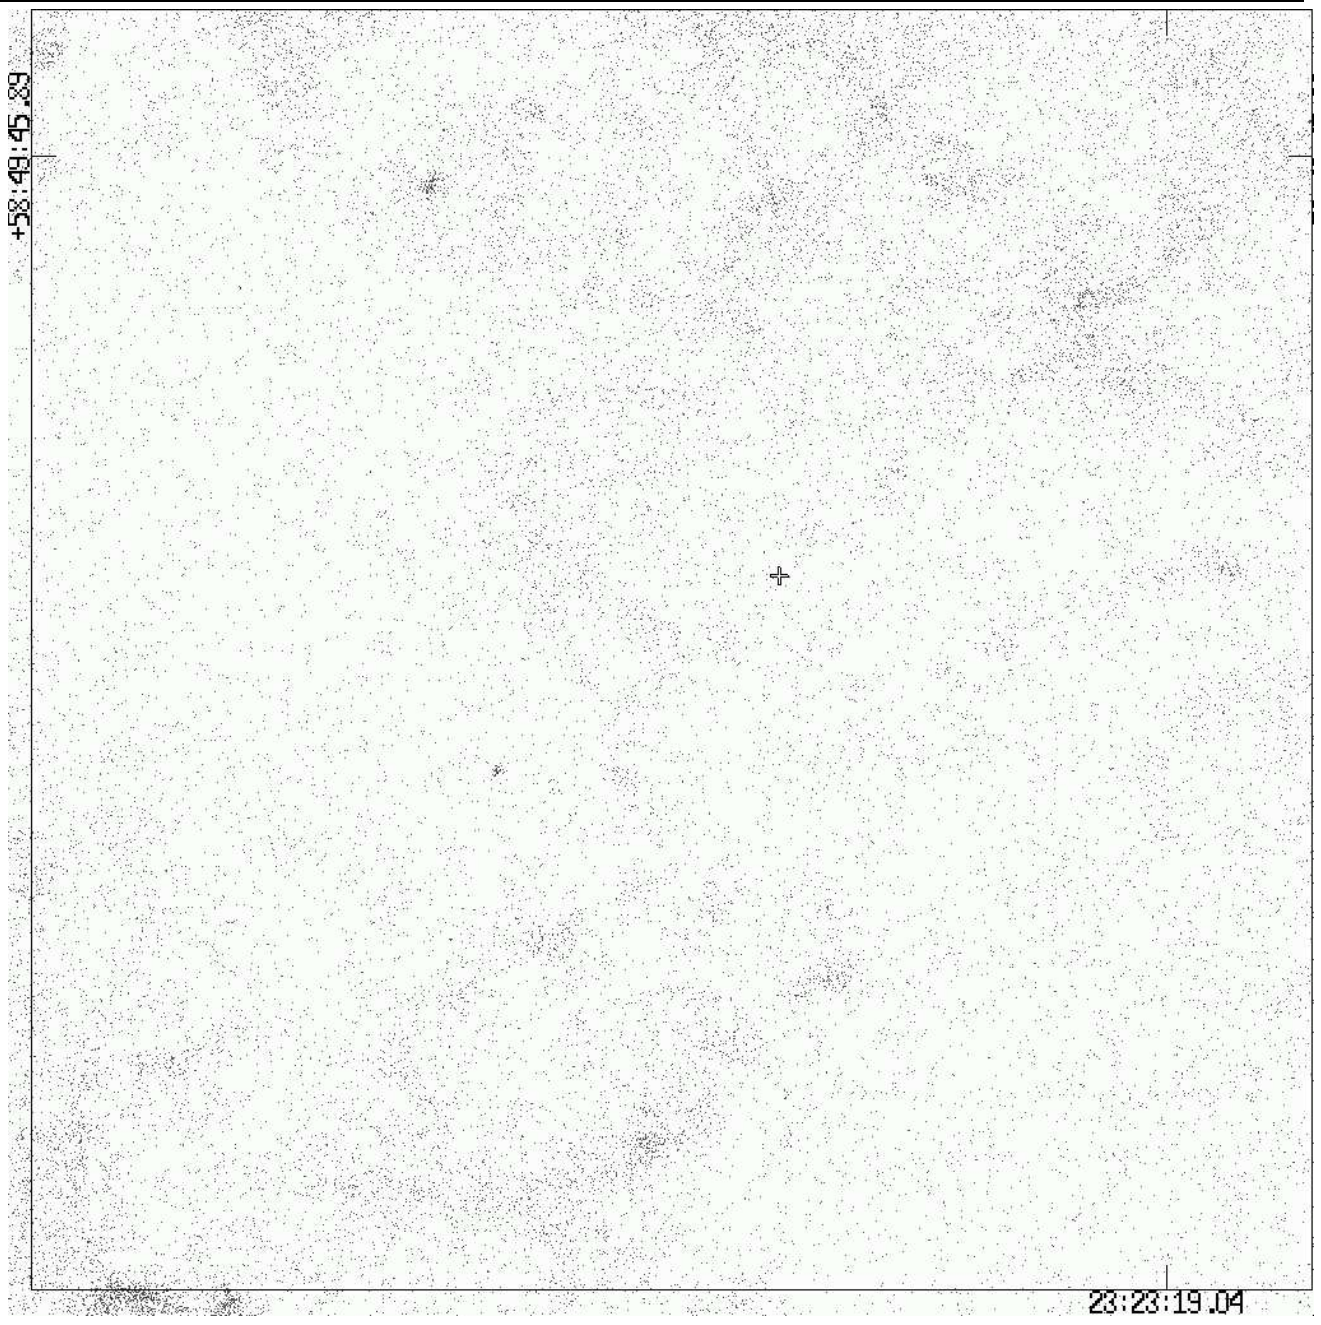

Chandra X-ray Center Seq Num: 590267

Instrument: HRC Obs ID: 2878

Source: CAS A [HRC-I, Offsets=0,0,0] PI: Dr. CXC Calibration

Title: AO3B CALIBRATION OBSERVATIONS THE STANDARD CANDLES CAS A AND G21.5-09

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.2	Processing system revision
DATE	2007-11-21T23:34:32	Date and time of file creation
DATE-OBS	2002-08-30T17:03:40	Observation start date
DATE-END	2002-08-30T18:39:19	Observation end date
RA_PNT	350.85077865407	Pointing RA
DEC_PNT	58.817362605089	Pointing Dec
ROLL_PNT	167.0912779754	Pointing Roll
RA_TARG	350.8575	Observer's specified target RA
DEC_TARG	58.814833	Observer's specified target Dec
DEGAP	hrciD1999-07-22gaplookupN0003.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.2	Processing system revision
DATE	2007-11-21T23:50:54	Date and time of file creation
DATE-OBS	2002-08-30T17:03:40	Observation start date
DATE-END	2002-08-30T18:39:19	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-I	Detector
GRATING	NONE	Grating
OBJECT	CAS A [HRC-I, Offsets=0,0,0]	Source name
TITLE	AO3B CALIBRATION OBSERVATIONS THE STANDARD CANDLES CAS A AND G21.5-09	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	2878	Observation id
SEQ_NUM	590267	Sequence number
RA_NOM	350.85077865407	Nominal RA
DEC_NOM	58.817362605089	Nominal Dec
ROLL_NOM	167.0912779754	Nominal Roll

Chandra X-ray Center

Seq Num: 590267

Instrument: HRC

Obs ID: 2878

Source: CAS A [HRC-I, Offsets=0,0,0]

PI: Dr. CXC Calibration

Title: AO3B CALIBRATION OBSERVATIONS THE STANDARD CANDLES CAS A AND G21.5-09

Full Field with Sources

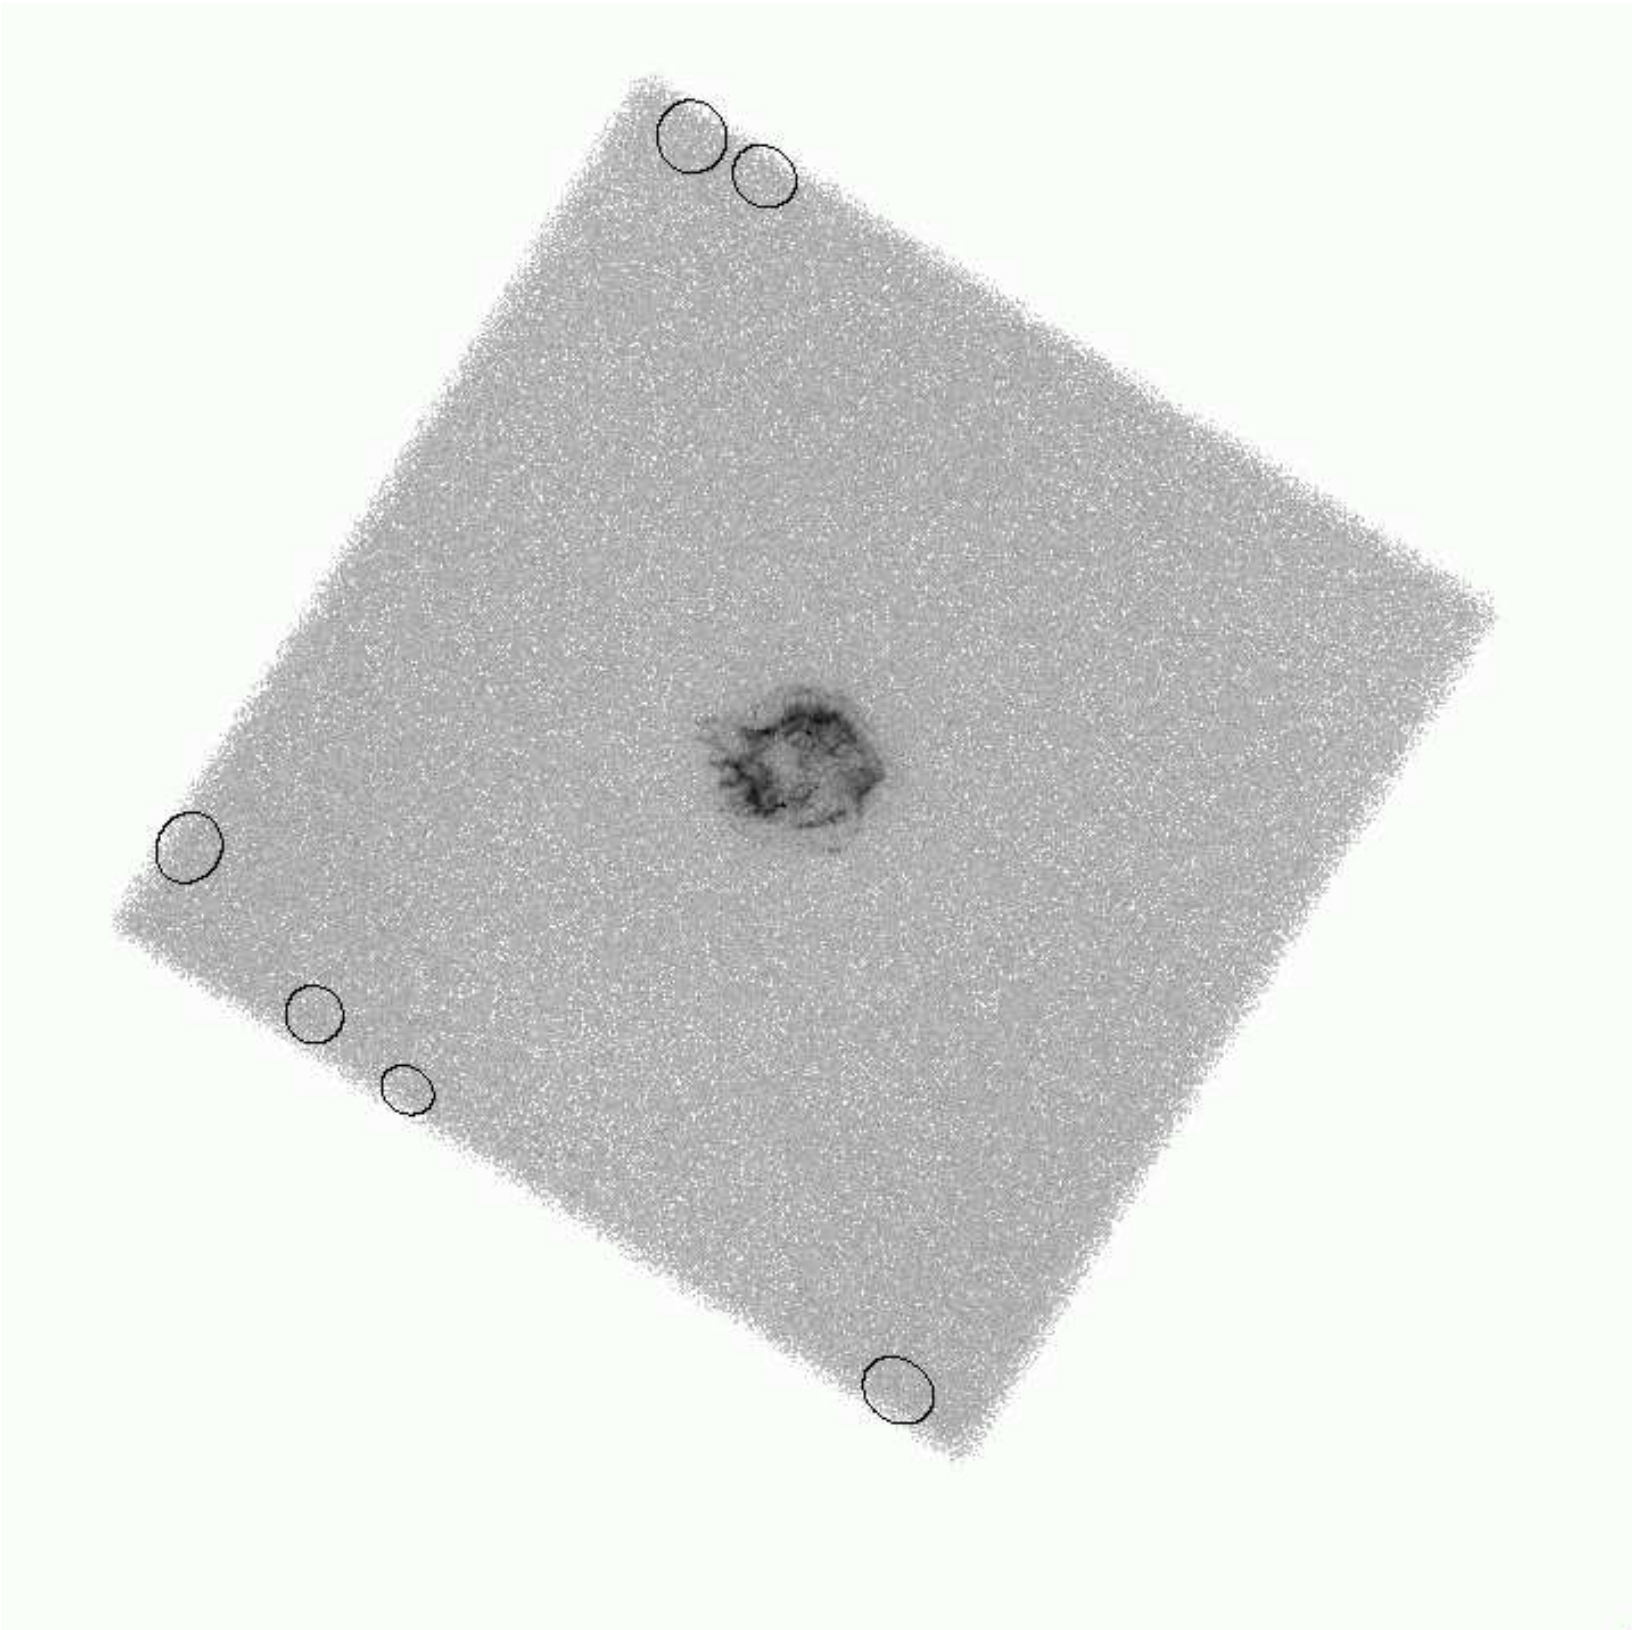

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
350.853012	58.840615	87.534088	15.103961	5.795439
350.768694	58.495183	248.428574	43.745564	5.678944
350.848380	58.839979	102.784088	19.280495	5.330988
350.974353	59.140122	228.262451	42.863945	5.325279
350.881306	58.796309	72.613640	14.624532	4.965194
351.346753	58.687626	171.208328	38.684555	4.425754
350.901568	59.119694	166.773209	37.867081	4.404174
351.472254	58.773007	193.225906	44.541096	4.338149
351.253983	58.649182	124.851746	29.224941	4.272096
350.857517	58.834228	50.833332	11.984953	4.241430