Chandra X-ray Center

Seq Num: 290244

Instrument: HRC

Obs ID: 3690

Source: VEGA

PI: Dr. CXC Calibration

Title: AO4 MEASUREMENTS OF THE OPTICAL/UV TRANSMISSION OF THE HRC AND ACIS FILTERS

---

hrcf03690N002 full img2.fits	hrcf03690N002 cntr img2.fits

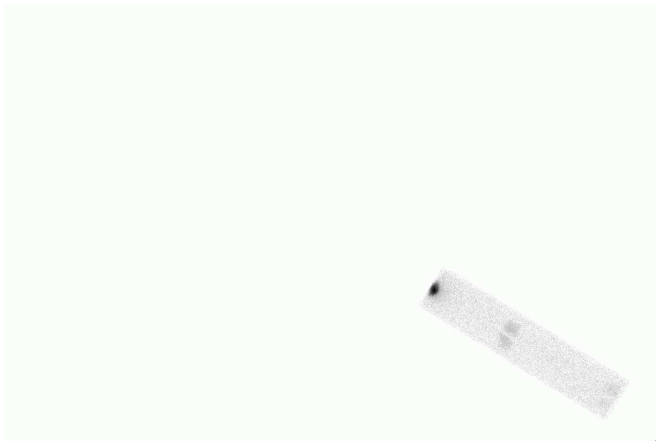

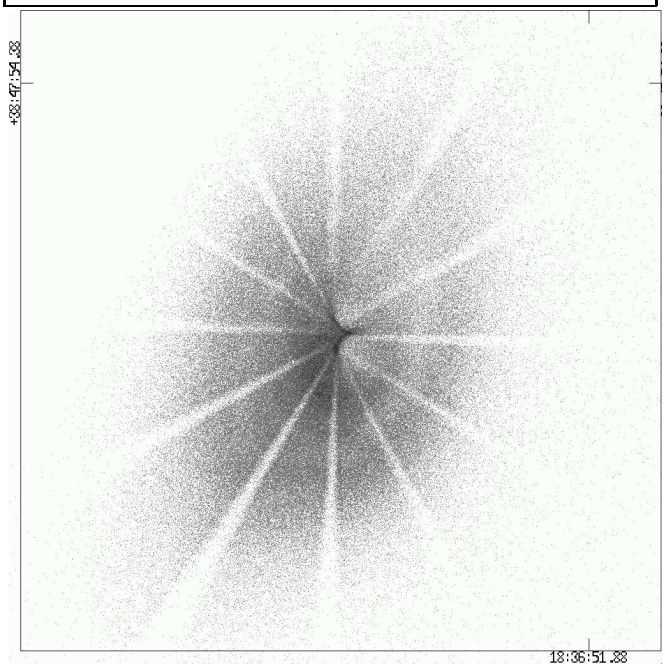

Chandra X-ray Center
Seq Num: 290244
Instrument: HRC
Obs ID: 3690
Source: VEGA
PI: Dr. CXC Calibration
Title: AO4 MEASUREMENTS OF THE OPTICAL/UV TRANSMISSION OF THE HRC AND ACIS FILTERS

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	Processing system revision
DATE	2006-07-19T13:28:25	Date and time of file creation
DATE-OBS	2003-01-27T06:26:03	Observation start date
DATE-END	2003-01-27T07:07:53	Observation end date
RA_PNT	279.60492928173	Pointing RA
DEC_PNT	38.960697682205	Pointing Dec
ROLL_PNT	31.578161422076	Pointing Roll
RA_TARG	279.235	Observer's specified target RA
DEC_TARG	38.783778	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	Processing system revision
DATE	2006-07-19T14:02:06	Date and time of file creation
DATE-OBS	2003-01-27T06:26:03	Observation start date
DATE-END	2003-01-27T07:07:53	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	NONE	Grating
OBJECT	VEGA	Source name
TITLE	AO4 MEASUREMENTS OF THE OPTICAL/UV TRANSMISSION OF THE HRC AND ACIS FILTERS	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	3690	Observation id
SEQ_NUM	290244	Sequence number
RA_NOM	279.60492928173	Nominal RA
DEC_NOM	38.960697682205	Nominal Dec
ROLL_NOM	31.578161422076	Nominal Roll

Chandra X-ray Center
Seq Num: 290244
Instrument: HRC
Obs ID: 3690
Source: VEGA
PI: Dr. CXC Calibration
Title: AO4 MEASUREMENTS OF THE OPTICAL/UV TRANSMISSION OF THE HRC AND ACIS FILTERS

Full Field with Sources

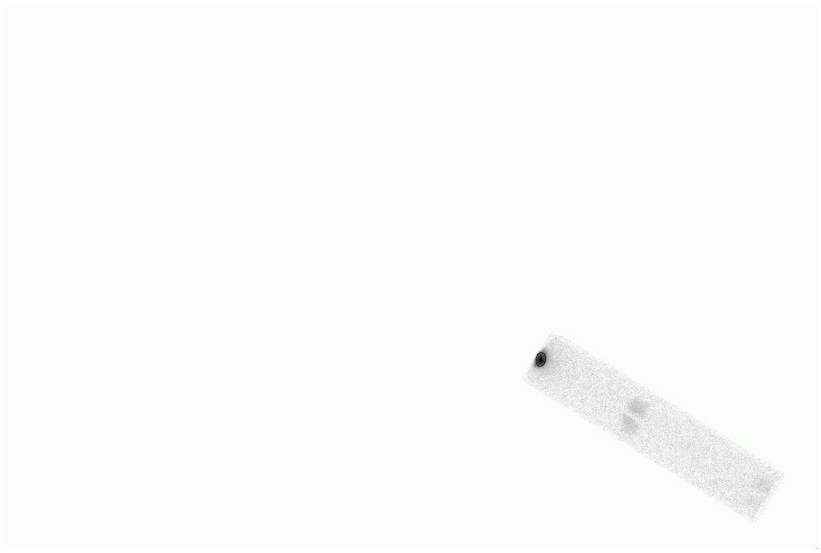

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
279.236714	38.782009	220975.359375	548.283142	403.031494