Chandra X-ray Center Seq Num: 590309

Instrument: ACIS Obs ID: 3697

Source: CAS A[S3,-120,-2.0,0,0] PI: Dr. CXC Calibration

Title: AO4A OBSERVATIONS OF THE STANDARD CANDLES CAS A AND G21.5-09

---

acisf03697N002 full img2.fits	acisf03697N002 cntr img2.fits

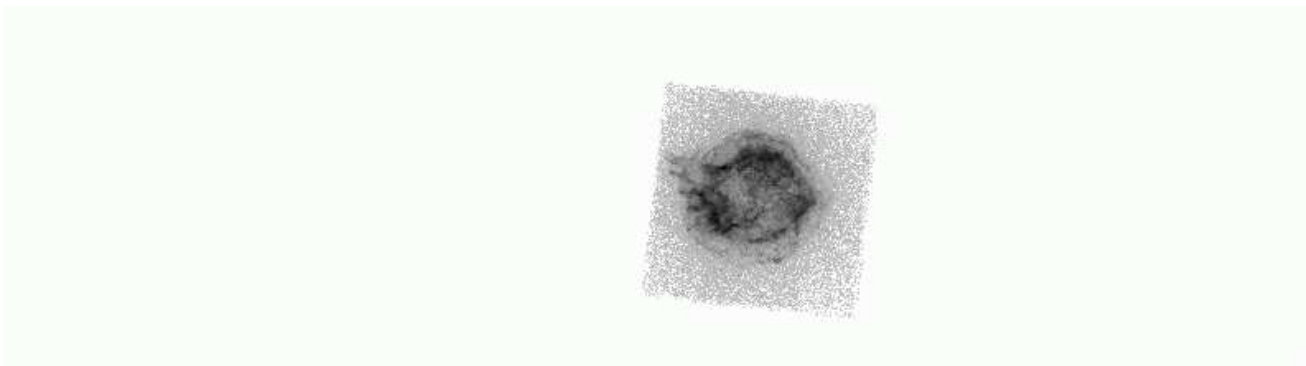

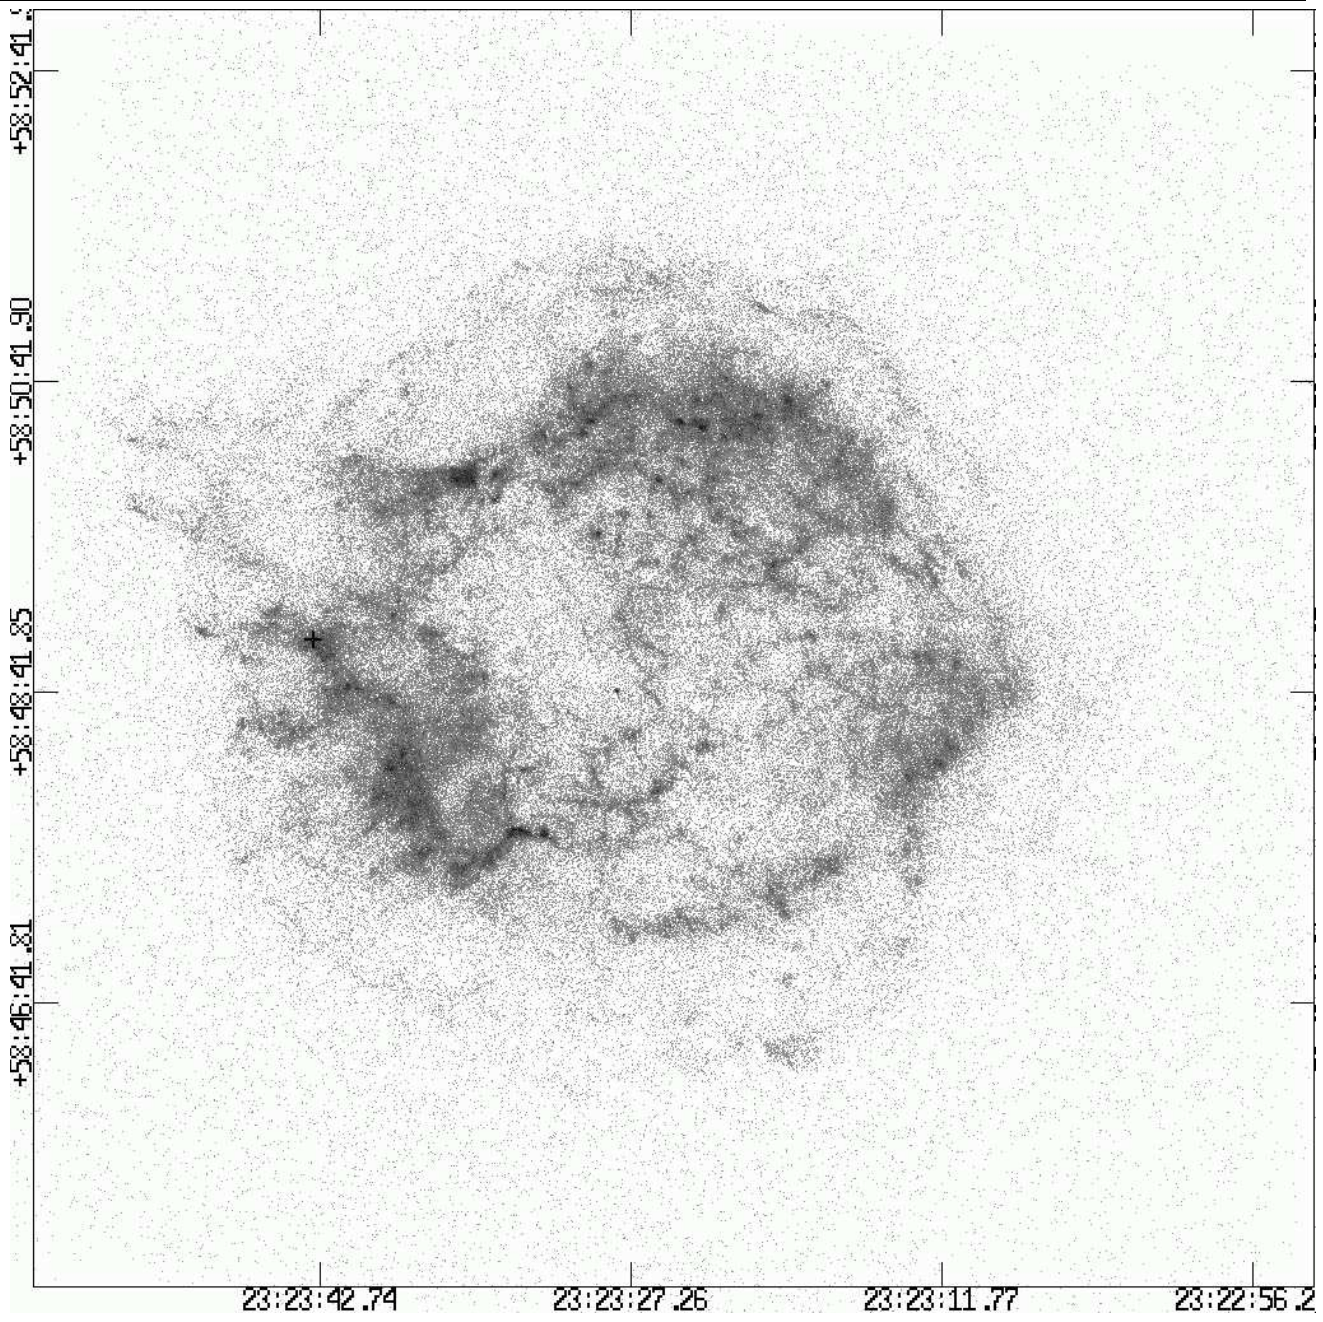

Chandra X-ray Center Seq Num: 590309

Instrument: ACIS Obs ID: 3697

Source: CAS A[S3,-120,-2.0,0,0] PI: Dr. CXC Calibration

Title: AO4A OBSERVATIONS OF THE STANDARD CANDLES CAS A AND G21.5-09

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-07-24T19:34:07	Date and time of file creation
DATE-OBS	2003-03-17T01:57:43	Observation start date
DATE-END	2003-03-17T03:01:40	Observation end date
RA_PNT	350.92940317221	Pointing RA
DEC_PNT	58.817221705302	Pointing Dec
ROLL_PNT	6.4285344258504	Pointing Roll
RA_TARG	350.8575	Observer's specified target RA
DEC_TARG	58.814833	Observer's specified target Dec
DATAMODE	FAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	153.76843262	Focal Plane Temperature [K]
FSW_VERS	30	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-07-24T20:16:06	Date and time of file creation
DATE-OBS	2003-03-17T01:57:43	Observation start date
DATE-END	2003-03-17T03:01:40	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-456789	Detector
GRATING	NONE	Grating
OBJECT	CAS A[S3,-120,-2.0,0,0]	Source name
TITLE	AO4A OBSERVATIONS OF THE STANDARD CANDLES CAS A AND G21.5-09	Propo
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	3697	Observation id
SEQ_NUM	590309	Sequence number
RA_NOM	350.92940317221	Nominal RA
DEC_NOM	58.817221705302	Nominal Dec
ROLL_NOM	6.4285344258504	Nominal Roll

Chandra X-ray Center

Seq Num: 590309

Instrument: ACIS

Obs ID: 3697

Source: CAS A[S3,-120,-2.0,0,0]

PI: Dr. CXC Calibration

Title: AO4A OBSERVATIONS OF THE STANDARD CANDLES CAS A AND G21.5-09

Full Field with Sources

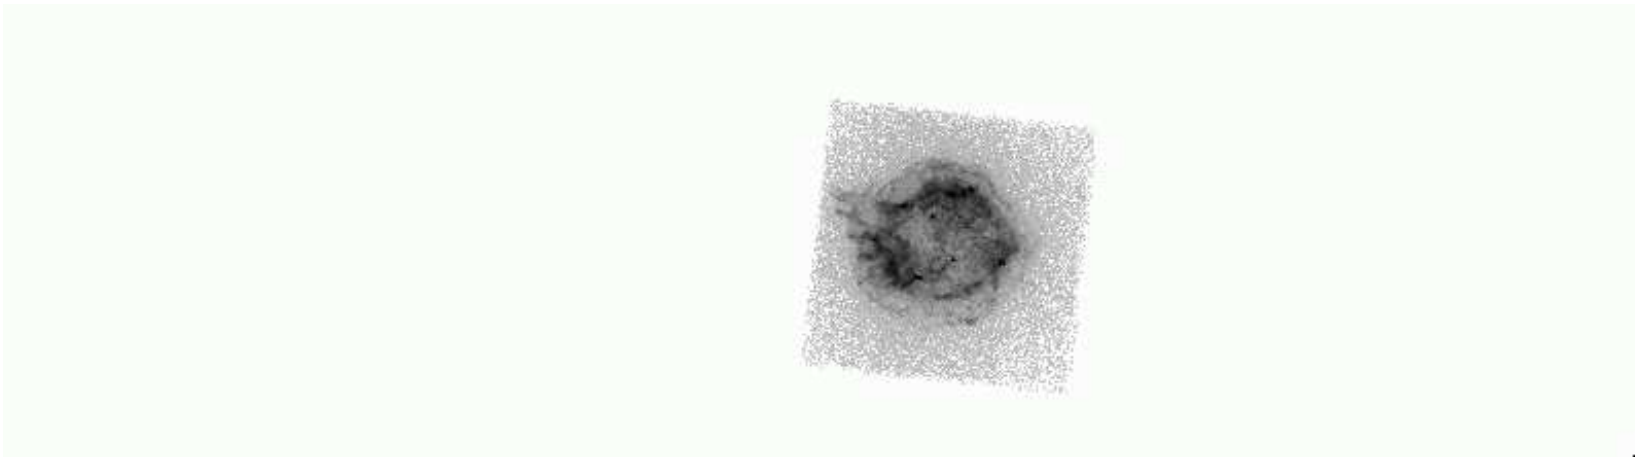

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
350.848495	58.840197	343.363647	34.640419	9.912226
350.853235	58.840613	293.931824	30.868050	9.522202
350.866426	58.811777	100.857140	13.064332	7.720038
350.881436	58.796424	197.571426	25.757402	7.670472
350.848434	58.805775	145.829544	19.867867	7.339970
350.799657	58.804014	250.714279	35.369190	7.088494
350.830964	58.843039	209.795456	30.526089	6.872661
350.837339	58.841371	199.113632	30.464855	6.535847
350.886172	58.796709	176.857147	27.755371	6.371997
350.870281	58.828499	121.857140	19.480944	6.255197