Chandra X-ray Center

Seq Num: 990004

Instrument: HRC

Obs ID: 4411

Source: ACIS BACKGROUND

PI: DR. CXC CALIBRATION

Title: AO4 CALIBRATION OBSERVATION TO MEASURE THE ACIS CHARGED PARTICLE BACKGROUND

---

hrcf04411N005 full img2.fits	hrcf04411N005 cntr img2.fits

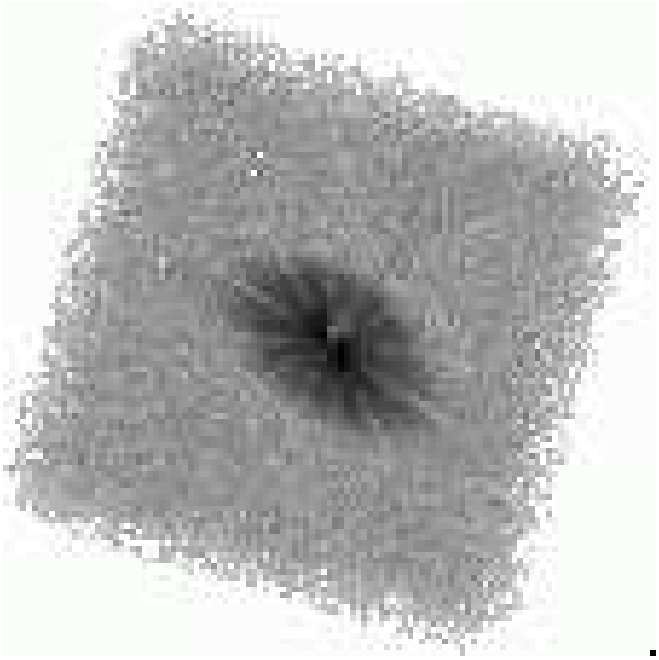

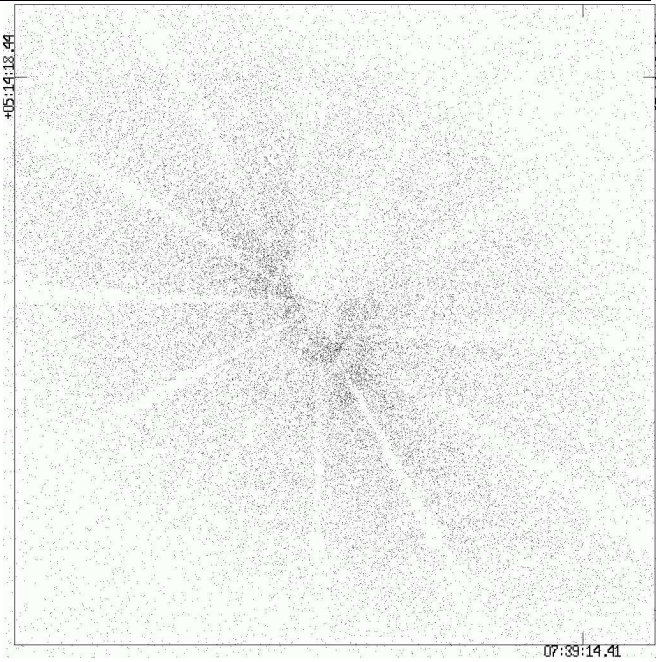

Chandra X-ray Center
Seq Num: 990004
Instrument: HRC
Obs ID: 4411
Source: ACIS BACKGROUND
PI: DR. CXC CALIBRATION
Title: AO4 CALIBRATION OBSERVATION TO MEASURE THE ACIS CHARGED PARTICLE BACKGROUND

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.10	Processing system revision
DATE	2009-02-05T00:16:42	Date and time of file creation
DATE-OBS	2003-12-08T08:43:34	Observation start date
DATE-END	2003-12-08T22:27:08	Observation end date
RA_PNT	115.06771465202	Pointing RA
DEC_PNT	4.8723758036508	Pointing Dec
ROLL_PNT	61.384542073677	Pointing Roll
RA_TARG	114.824708	Observer's specified target RA
DEC_TARG	5.223861	Observer's specified target Dec
DEGAP	hrciD1999-07-22gaplookupN0003.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.10	Processing system revision
DATE	2009-02-05T01:32:52	Date and time of file creation
DATE-OBS	2003-12-08T08:43:34	Observation start date
DATE-END	2003-12-08T22:27:08	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-I	Detector
GRATING	NONE	Grating
OBJECT	ACIS BACKGROUND	Source name
TITLE	AO4 CALIBRATION OBSERVATION TO MEASURE THE ACIS CHARGED PARTICLE BACKGROUND	Proposal title
OBSERVER	DR. CXC CALIBRATION	Principal investigator
OBS_ID	4411	Observation id
SEQ_NUM	990004	Sequence number
RA_NOM	115.06771465202	Nominal RA
DEC_NOM	4.8723758036508	Nominal Dec
ROLL_NOM	61.384542073677	Nominal Roll

Chandra X-ray Center
Seq Num: 990004
Instrument: HRC
Obs ID: 4411
Source: ACIS BACKGROUND
PI: DR. CXC CALIBRATION
Title: AO4 CALIBRATION OBSERVATION TO MEASURE THE ACIS CHARGED PARTICLE BACKGROUND

Full Field with Sources

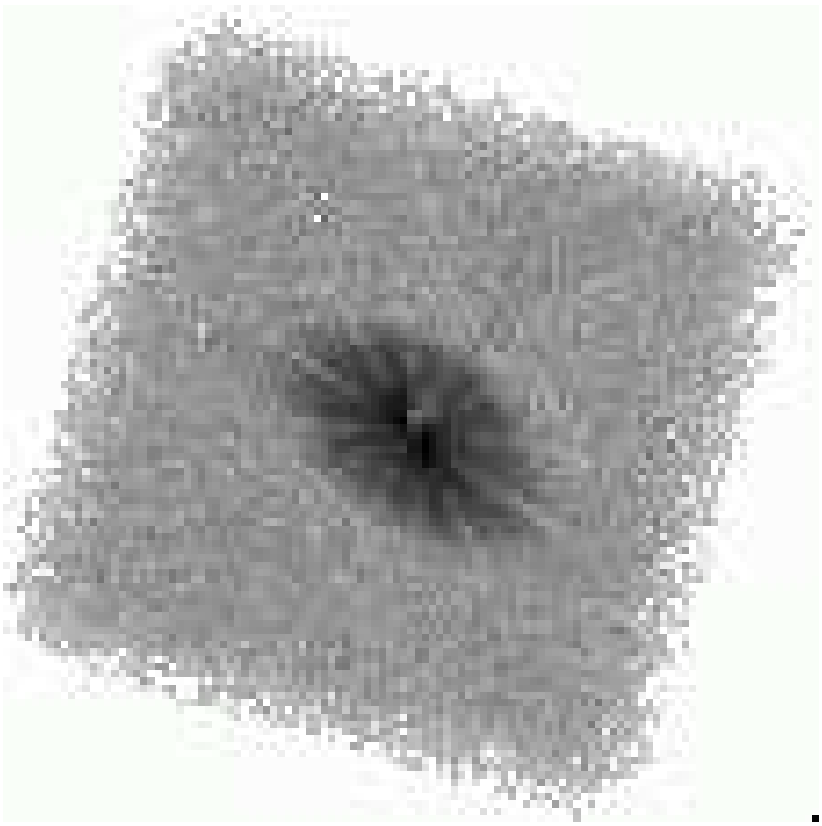

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR