Summary Page Created:Sun June 4, 2006 07:18 EDT

Chandra X-ray Center

Seq Num: 290324

Instrument: HRC

Obs ID: 5051

Source: Vega

PI: Dr. CXC Calibration

Title: AO5 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

---

hrcf05051N002 full img2.fits

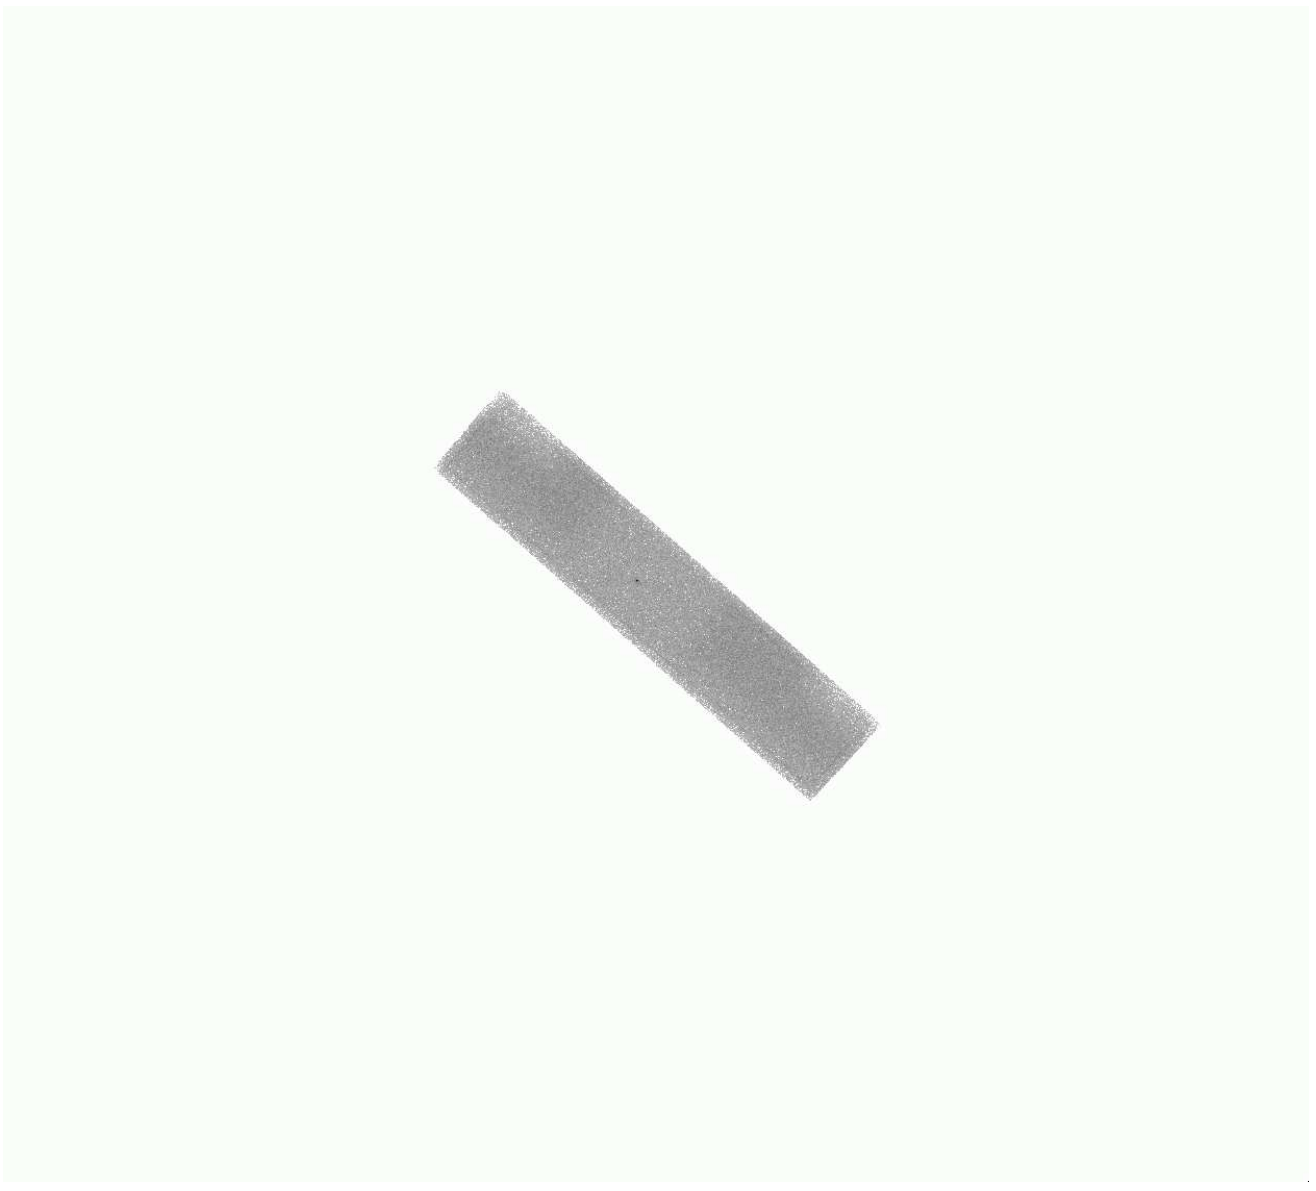

hrcf05051N002 cntr img2.fits

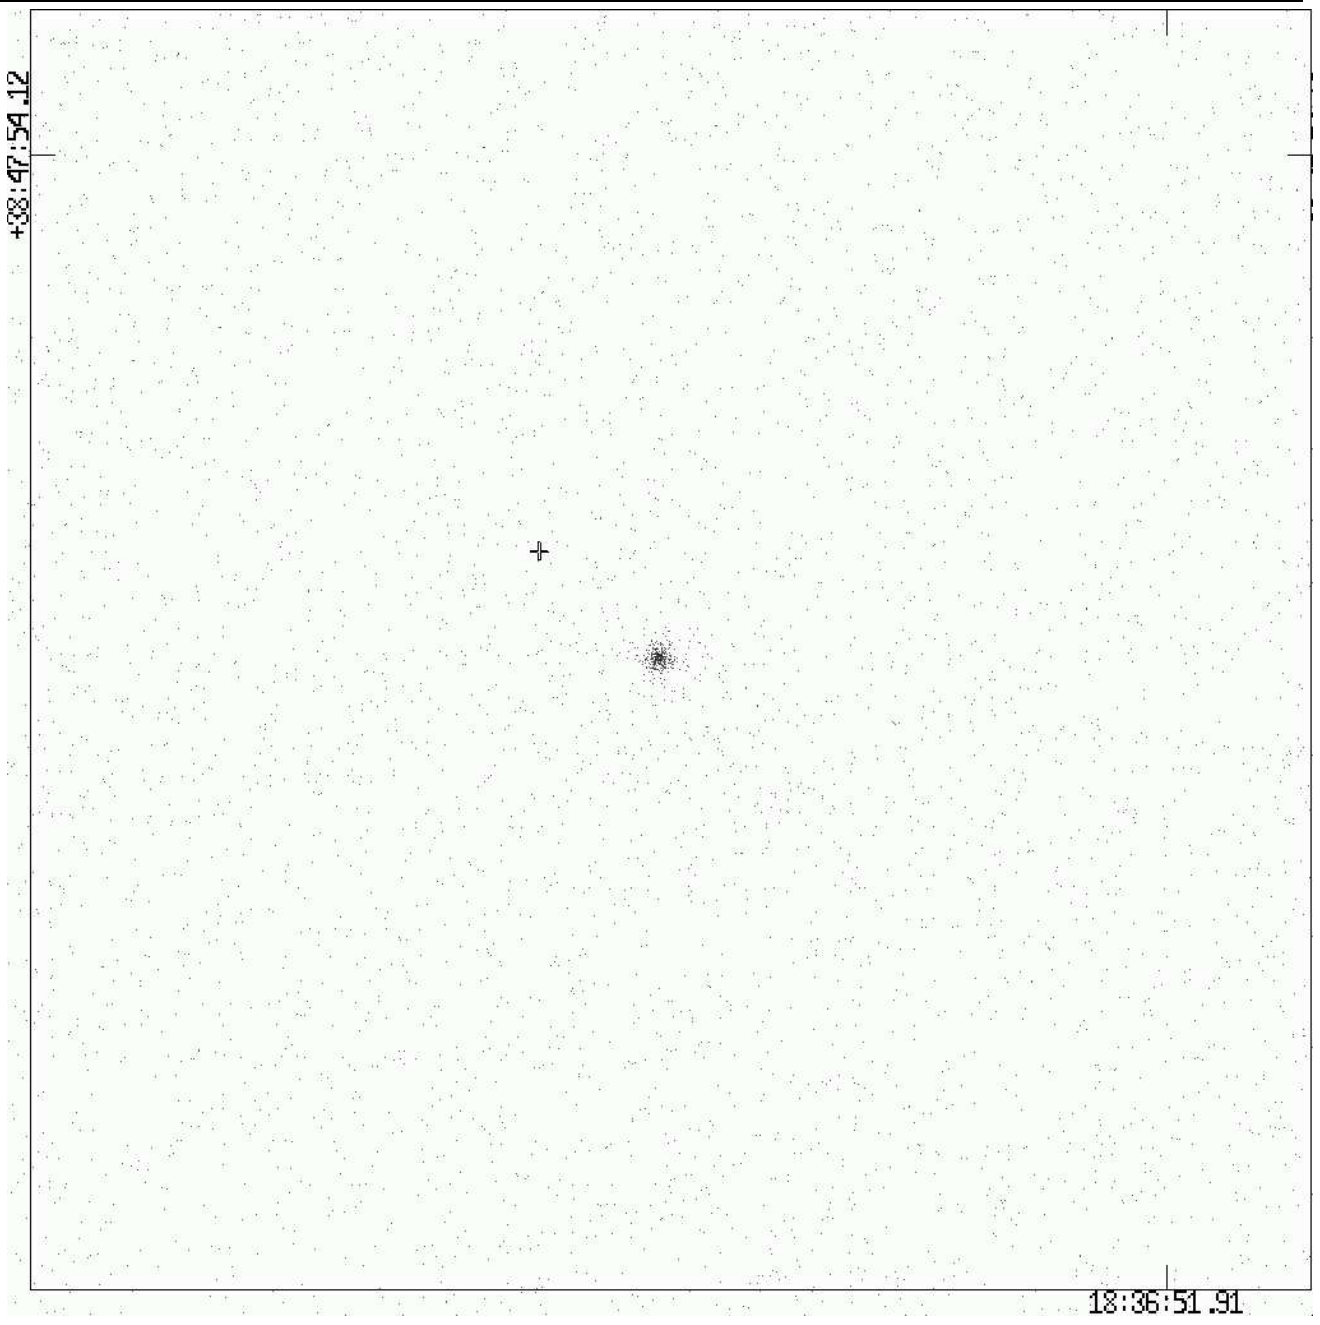

Chandra X-ray Center Seq Num: 290324
Instrument: HRC Obs ID: 5051
Source: Vega PI: Dr. CXC Calibration
Title: AO5 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.2	Processing system revision
DATE	2006-06-04T10:31:53	Date and time of file creation
DATE-OBS	2004-02-05T02:22:51	Observation start date
DATE-END	2004-02-05T03:04:40	Observation end date
RA_PNT	279.23937026076	Pointing RA
DEC_PNT	38.786994048816	Pointing Dec
ROLL_PNT	41.332818069578	Pointing Roll
RA_TARG	279.235	Observer's specified target RA
DEC_TARG	38.783778	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.2	Processing system revision
DATE	2006-06-04T11:16:46	Date and time of file creation
DATE-OBS	2004-02-05T02:22:51	Observation start date
DATE-END	2004-02-05T03:04:40	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	NONE	Grating
OBJECT	Vega	Source name
TITLE	AO5 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5051	Observation id
SEQ_NUM	290324	Sequence number
RA_NOM	279.23937026076	Nominal RA
DEC_NOM	38.786994048816	Nominal Dec
ROLL_NOM	41.332818069578	Nominal Roll

Chandra X-ray Center Seq Num: 290324

Instrument: HRC Obs ID: 5051

Source: Vega PI: Dr. CXC Calibration

Title: AO5 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

Full Field with Sources

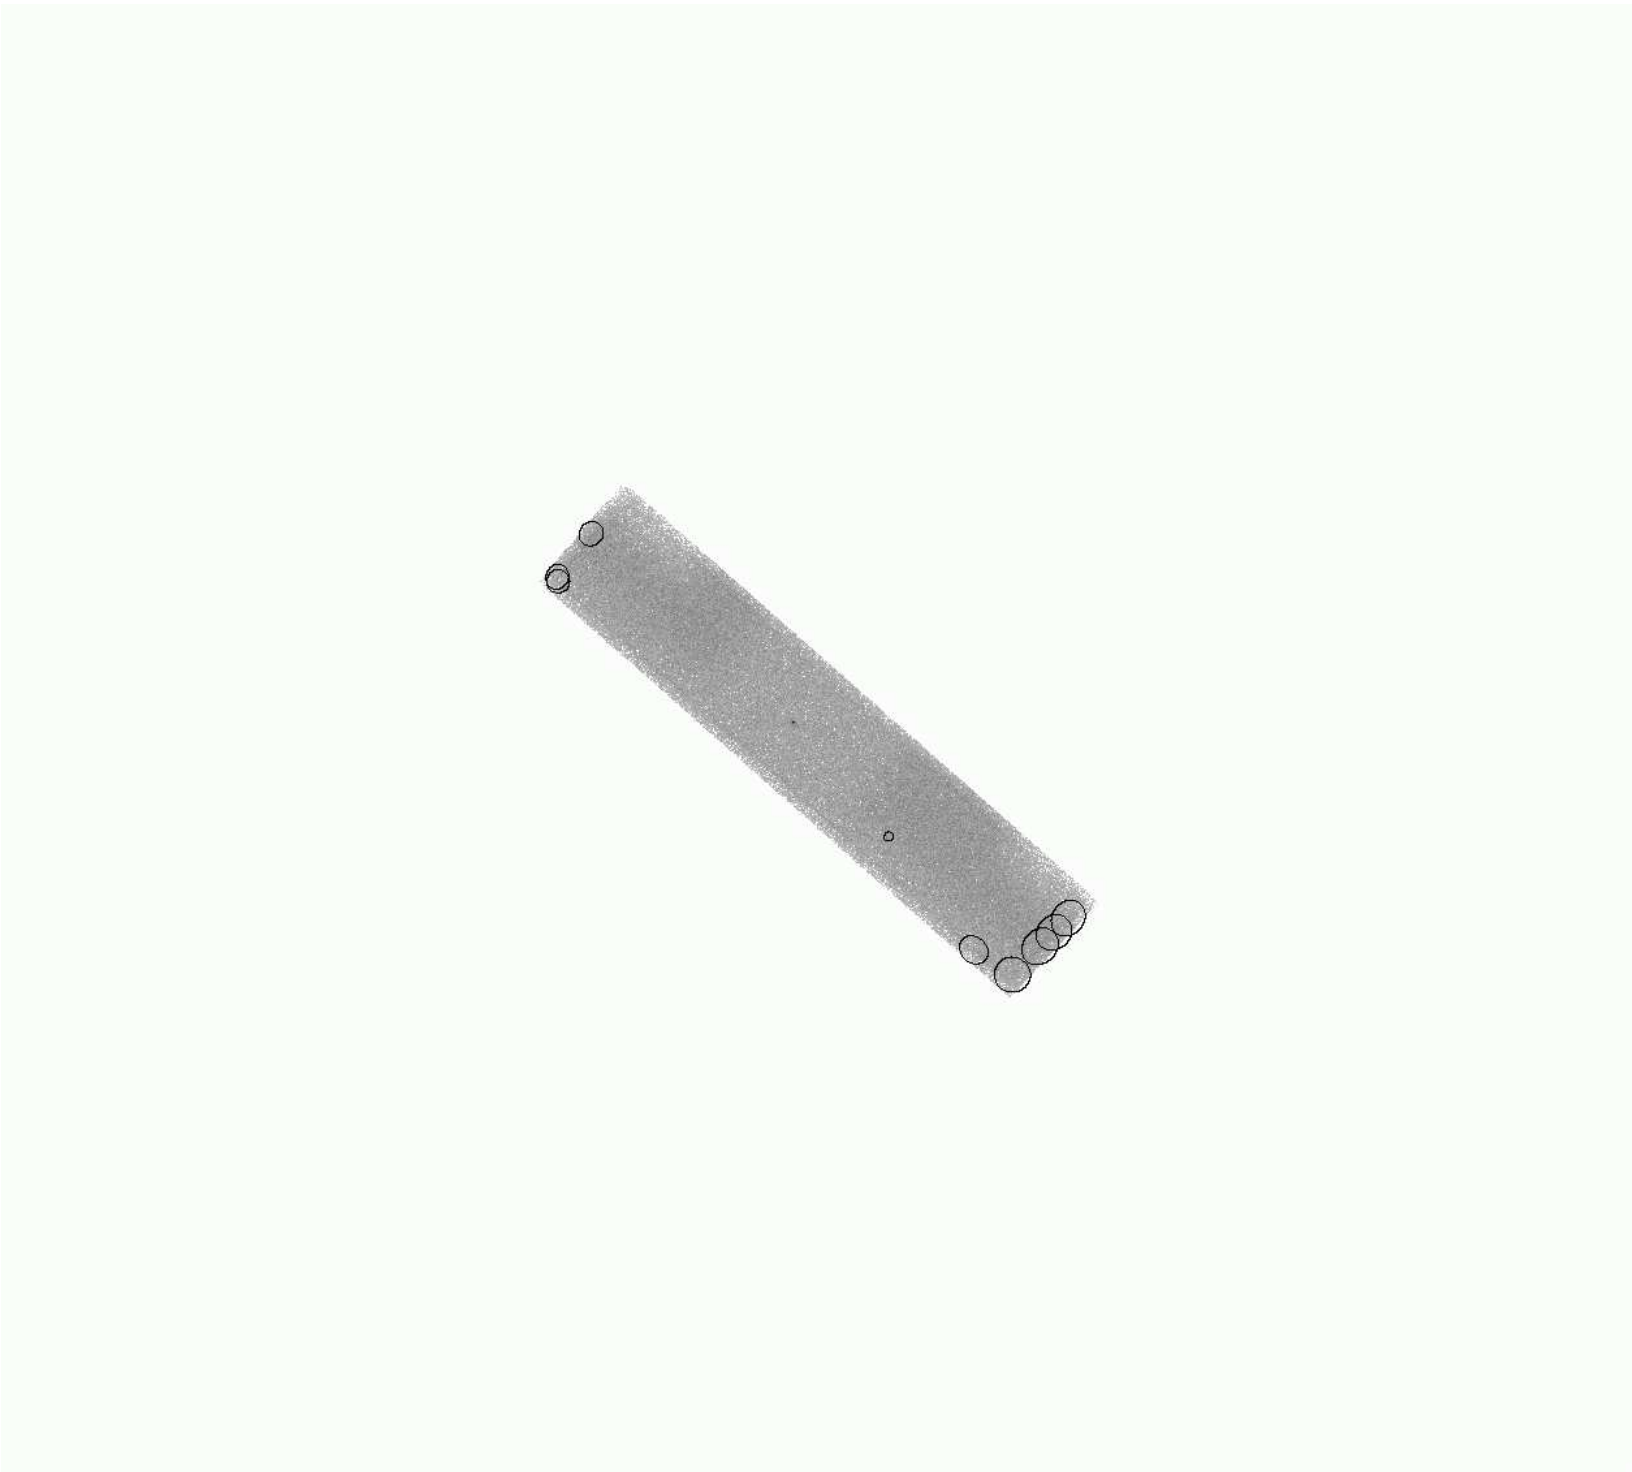

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
279.234929	38.783919	117.375000	17.304516	6.782911
278.951488	38.581523	304.363403	50.480091	6.029375
278.935352	38.594088	272.090179	49.237335	5.526095
278.919059	38.606821	229.620529	42.132736	5.449932
278.983407	38.556185	222.810715	43.051254	5.175476
279.508668	38.914188	118.000000	28.494772	4.141110
279.027791	38.578592	129.135635	32.623142	3.958406
279.469587	38.952967	120.708336	33.935486	3.556995
279.125797	38.680651	50.799107	14.683743	3.459548
279.507637	38.910139	93.960785	27.268627	3.445747