Chandra X-ray Center

Seq Num: 590324

Instrument: ACIS

Obs ID: 5126

Source: E0102-72[S0,-120,21.44,0,0]

PI: Dr. CXC Calibration

Title: AO5A ACIS-S Calibration Observations of E0102-72

---

acisf05126N002 full img2.fits

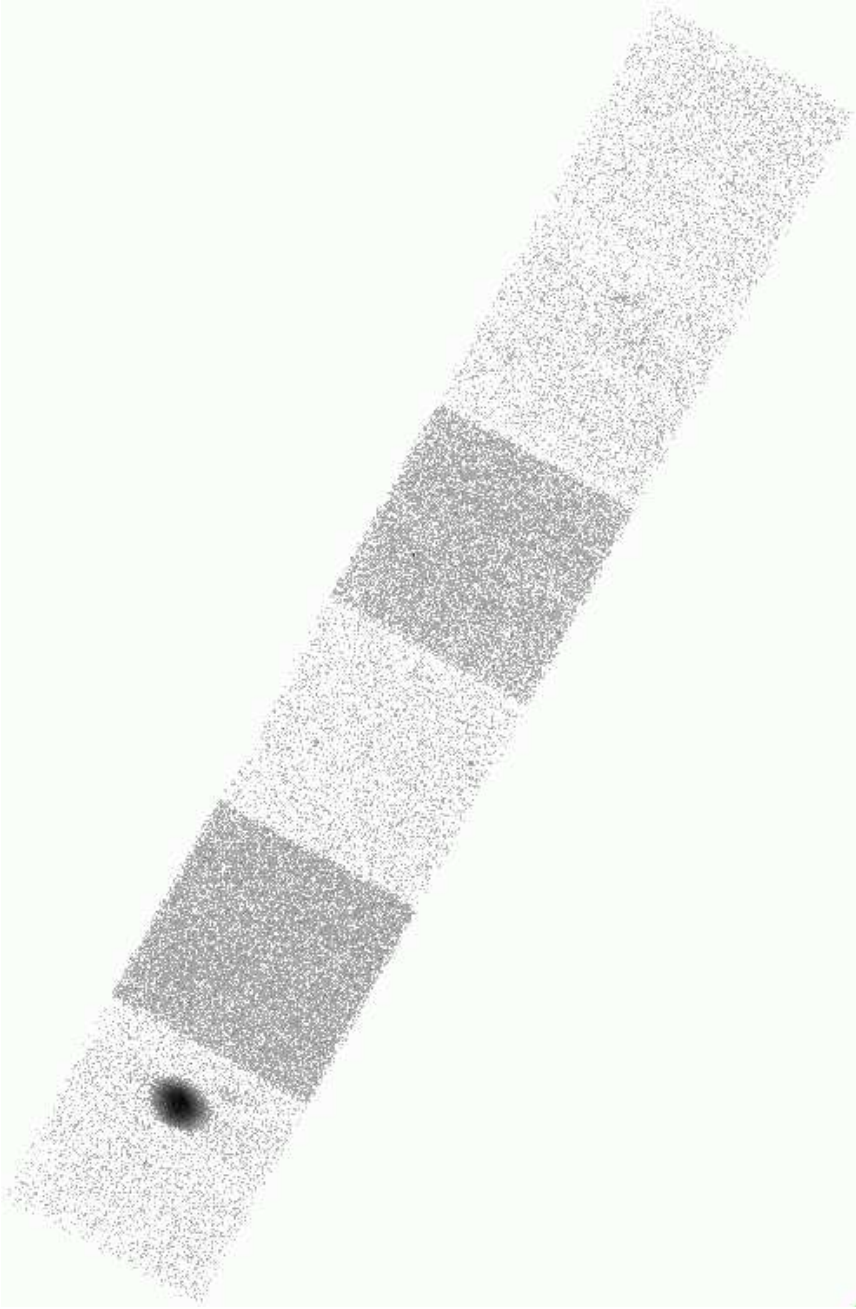

acisf05126N002 cntr img2.fits

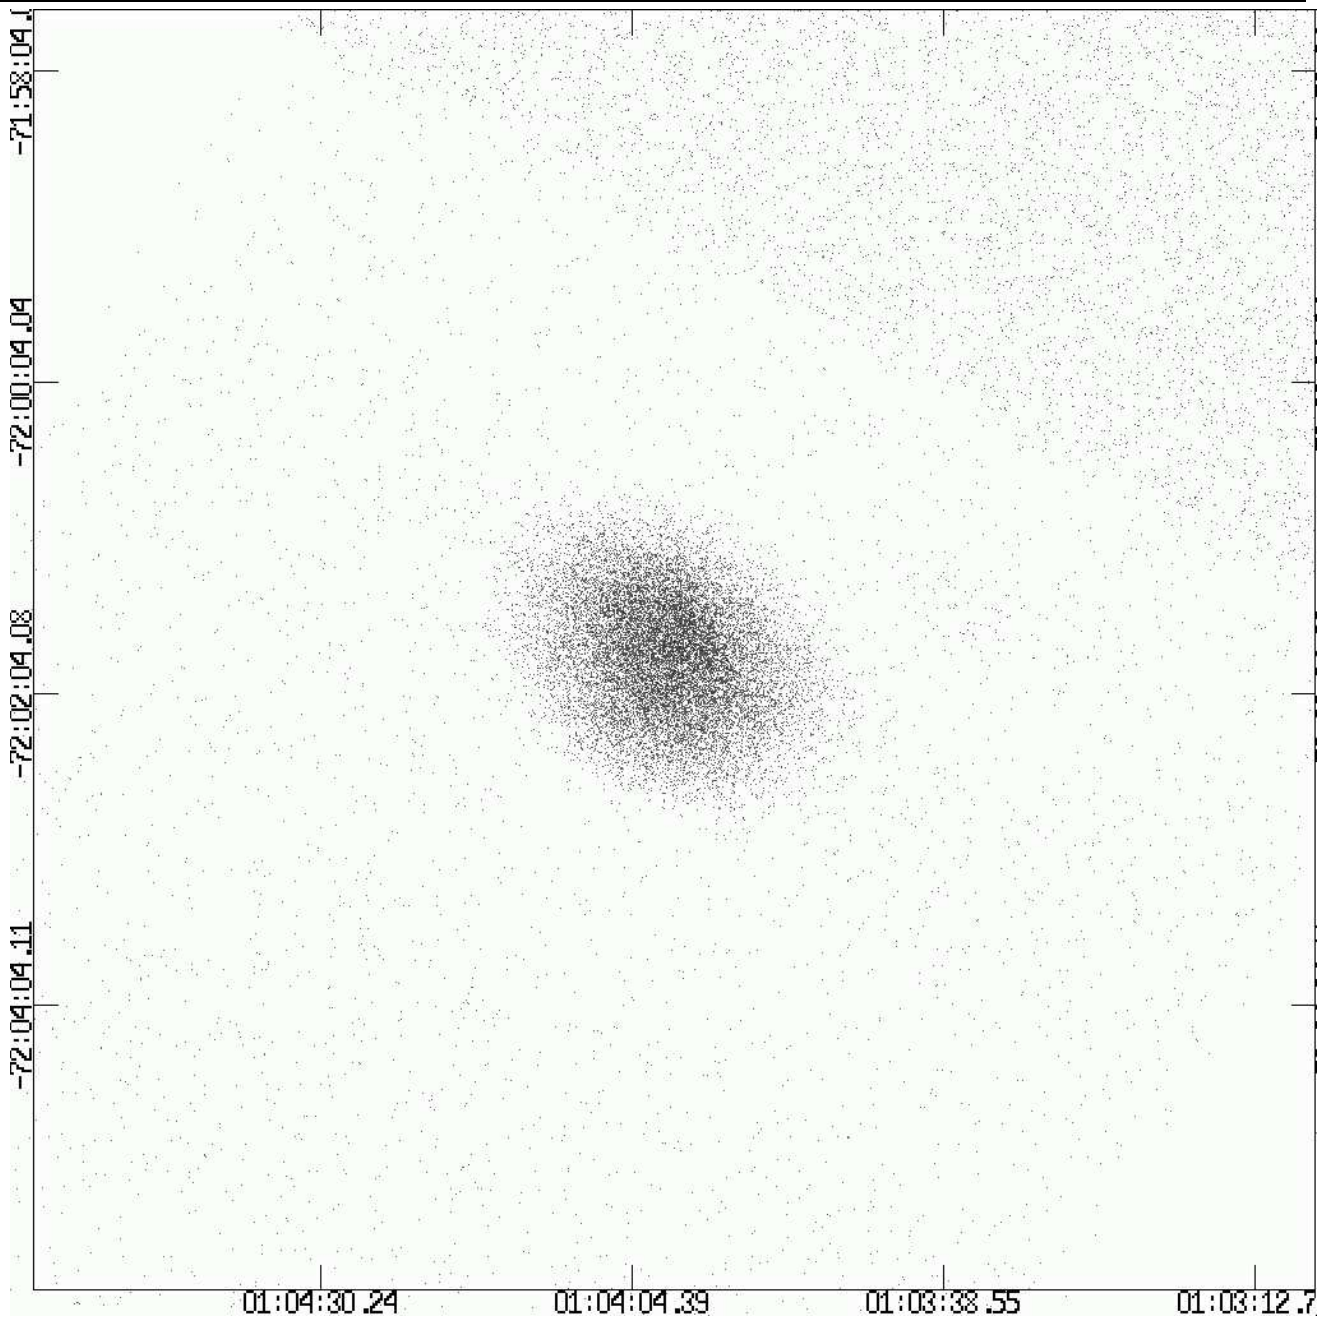

Chandra X-ray Center Seq Num: 590324

Instrument: ACIS Obs ID: 5126

Source: E0102-72[S0,-120,21.44,0,0] PI: Dr. CXC Calibration

Title: AO5A ACIS-S Calibration Observations of E0102-72

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-06-23T17:06:16	Date and time of file creation
DATE-OBS	2003-12-15T15:25:02	Observation start date
DATE-END	2003-12-15T17:51:02	Observation end date
RA_PNT	15.455382555346	Pointing RA
DEC_PNT	-71.723607825018	Pointing Dec
ROLL_PNT	298.84218135993	Pointing Roll
RA_TARG	16.01	Observer's specified target RA
DEC_TARG	-72.032028	Observer's specified target Dec
DATAMODE	VFAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	153.4460144	Focal Plane Temperature [K]
FSW_VERS	30	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-06-23T17:20:38	Date and time of file creation
DATE-OBS	2003-12-15T15:25:02	Observation start date
DATE-END	2003-12-15T17:51:02	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-456789	Detector
GRATING	NONE	Grating
OBJECT	E0102-72[S0,-120,21.44,0,0]	Source name
TITLE	AO5A ACIS-S Calibration Observations of E0102-72	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5126	Observation id
SEQ_NUM	590324	Sequence number
RA_NOM	15.455382555346	Nominal RA
DEC_NOM	-71.723607825018	Nominal Dec
ROLL_NOM	298.84218135993	Nominal Roll

Chandra X-ray Center

Seq Num: 590324

Instrument: ACIS

Obs ID: 5126

Source: E0102-72[S0,-120,21.44,0,0]

PI: Dr. CXC Calibration

Title: AO5A ACIS-S Calibration Observations of E0102-72

Full Field with Sources

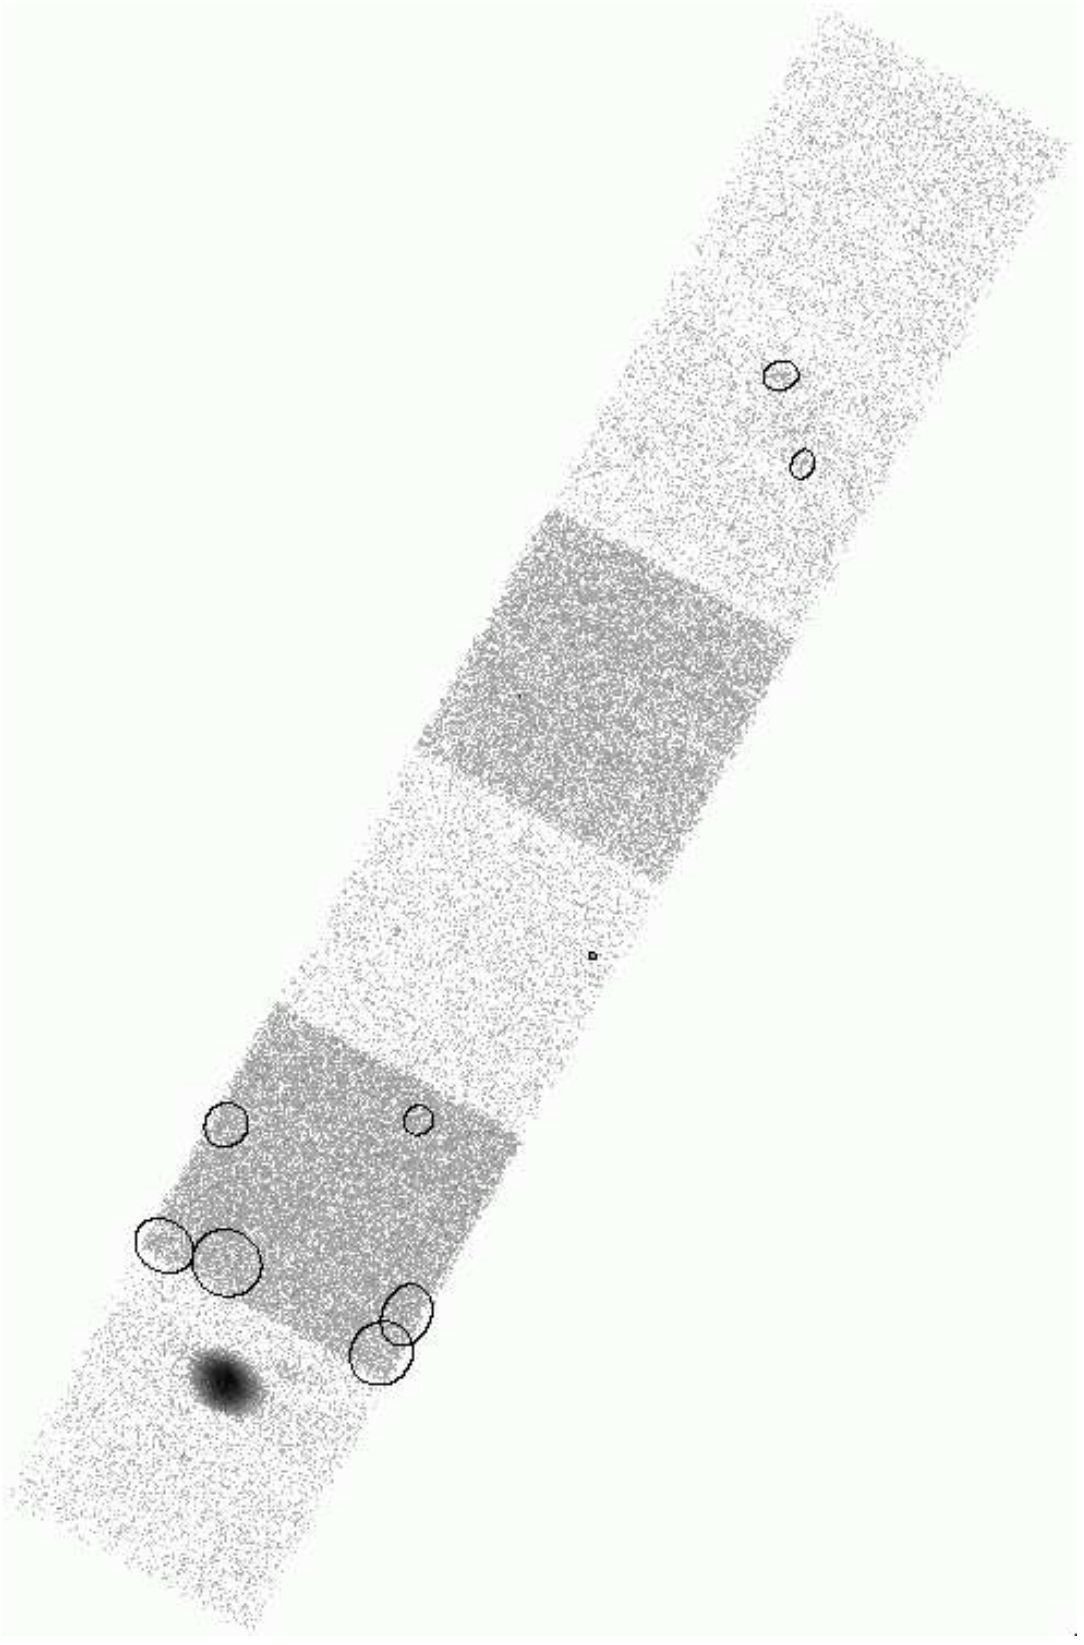

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
15.527853	-71.687794	71.714287	10.042165	7.141317
16.106479	-71.962731	113.767441	22.523300	5.051100
15.714345	-71.998385	112.947319	25.797899	4.378160
15.755285	-72.017506	112.425247	26.522785	4.238818
15.115830	-71.527137	42.728722	11.032840	3.872867
15.080399	-71.571553	25.708334	7.867955	3.267473
16.005025	-71.971659	100.867111	30.907759	3.263488
15.412553	-71.818459	19.897499	6.215782	3.201126
16.003992	-71.902413	64.041382	20.494091	3.124870
15.693348	-71.900783	47.166668	15.336946	3.075362