Chandra X-ray Center

Seq Num: 590342

Instrument: ACIS

Obs ID: 5144

Source: E0102-72[I1,-120,-4.0,-3.68,0]

PI: Dr. CXC Calibration

Title: AO5B ACIS-I Calibration Observations of E0102-72

---

acisf05144N002 full img2.fits	acisf05144N002 cntr img2.fits

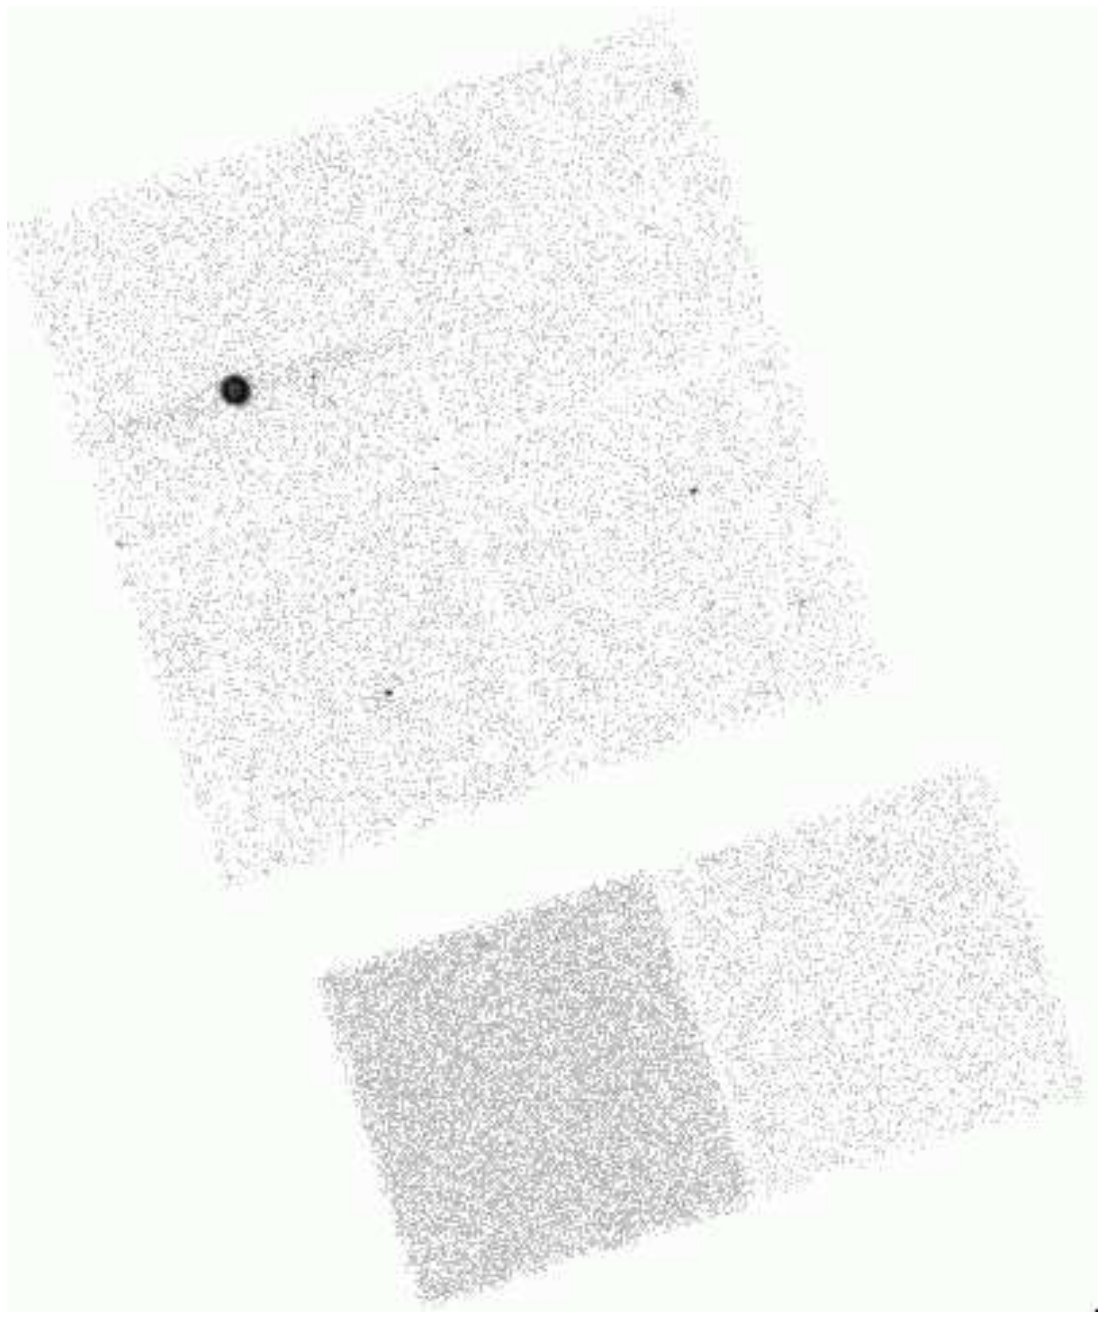

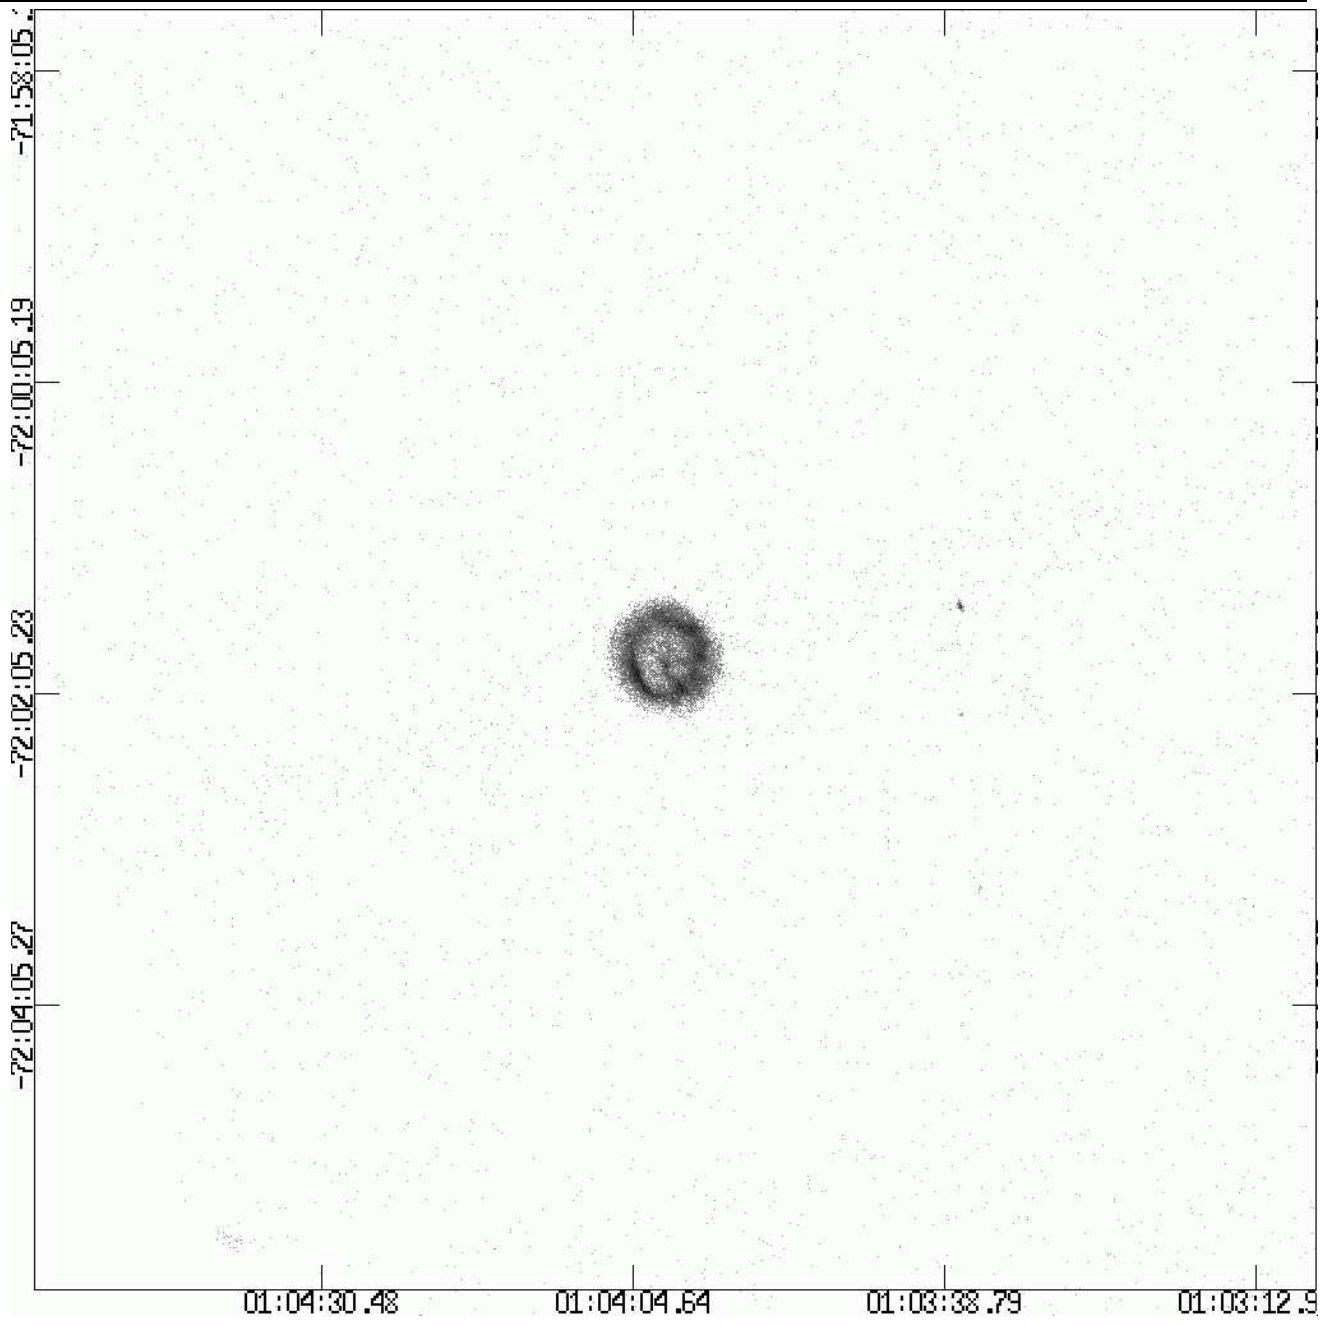

Chandra X-ray Center
Seq Num: 590342

Instrument: ACIS
Obs ID: 5144

Source: E0102-72[I1,-120,-4.0,-3.68,0]
PI: Dr. CXC Calibration

Title: AO5B ACIS-I Calibration Observations of E0102-72

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.2	ASCDS version number
DATE	2006-05-20T10:32:34	Date and time of file creation
DATE-OBS	2004-04-26T13:14:29	Observation start date
DATE-END	2004-04-26T15:27:40	Observation end date
RA_PNT	15.731506676475	Pointing RA
DEC_PNT	-72.066866681074	Pointing Dec
ROLL_PNT	162.1708352239	Pointing Roll
RA_TARG	16.01	Observer's specified target RA
DEC_TARG	-72.032028	Observer's specified target Dec
DATAMODE	VFAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	153.4460144	Focal Plane Temperature [K]
FSW_VERS	30	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.2	ASCDS version number
DATE	2006-05-20T10:59:12	Date and time of file creation
DATE-OBS	2004-04-26T13:14:29	Observation start date
DATE-END	2004-04-26T15:27:40	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-012367	Detector
GRATING	NONE	Grating
OBJECT	E0102-72[I1,-120,-4.0,-3.68,0]	Source name
TITLE	AO5B ACIS-I Calibration Observations of E0102-72	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5144	Observation id
SEQ_NUM	590342	Sequence number
RA_NOM	15.731506676475	Nominal RA
DEC_NOM	-72.066866681074	Nominal Dec
ROLL_NOM	162.1708352239	Nominal Roll

Chandra X-ray Center

Seq Num: 590342

Instrument: ACIS

Obs ID: 5144

Source: E0102-72[I1,-120,-4.0,-3.68,0]

PI: Dr. CXC Calibration

Title: AO5B ACIS-I Calibration Observations of E0102-72

Full Field with Sources

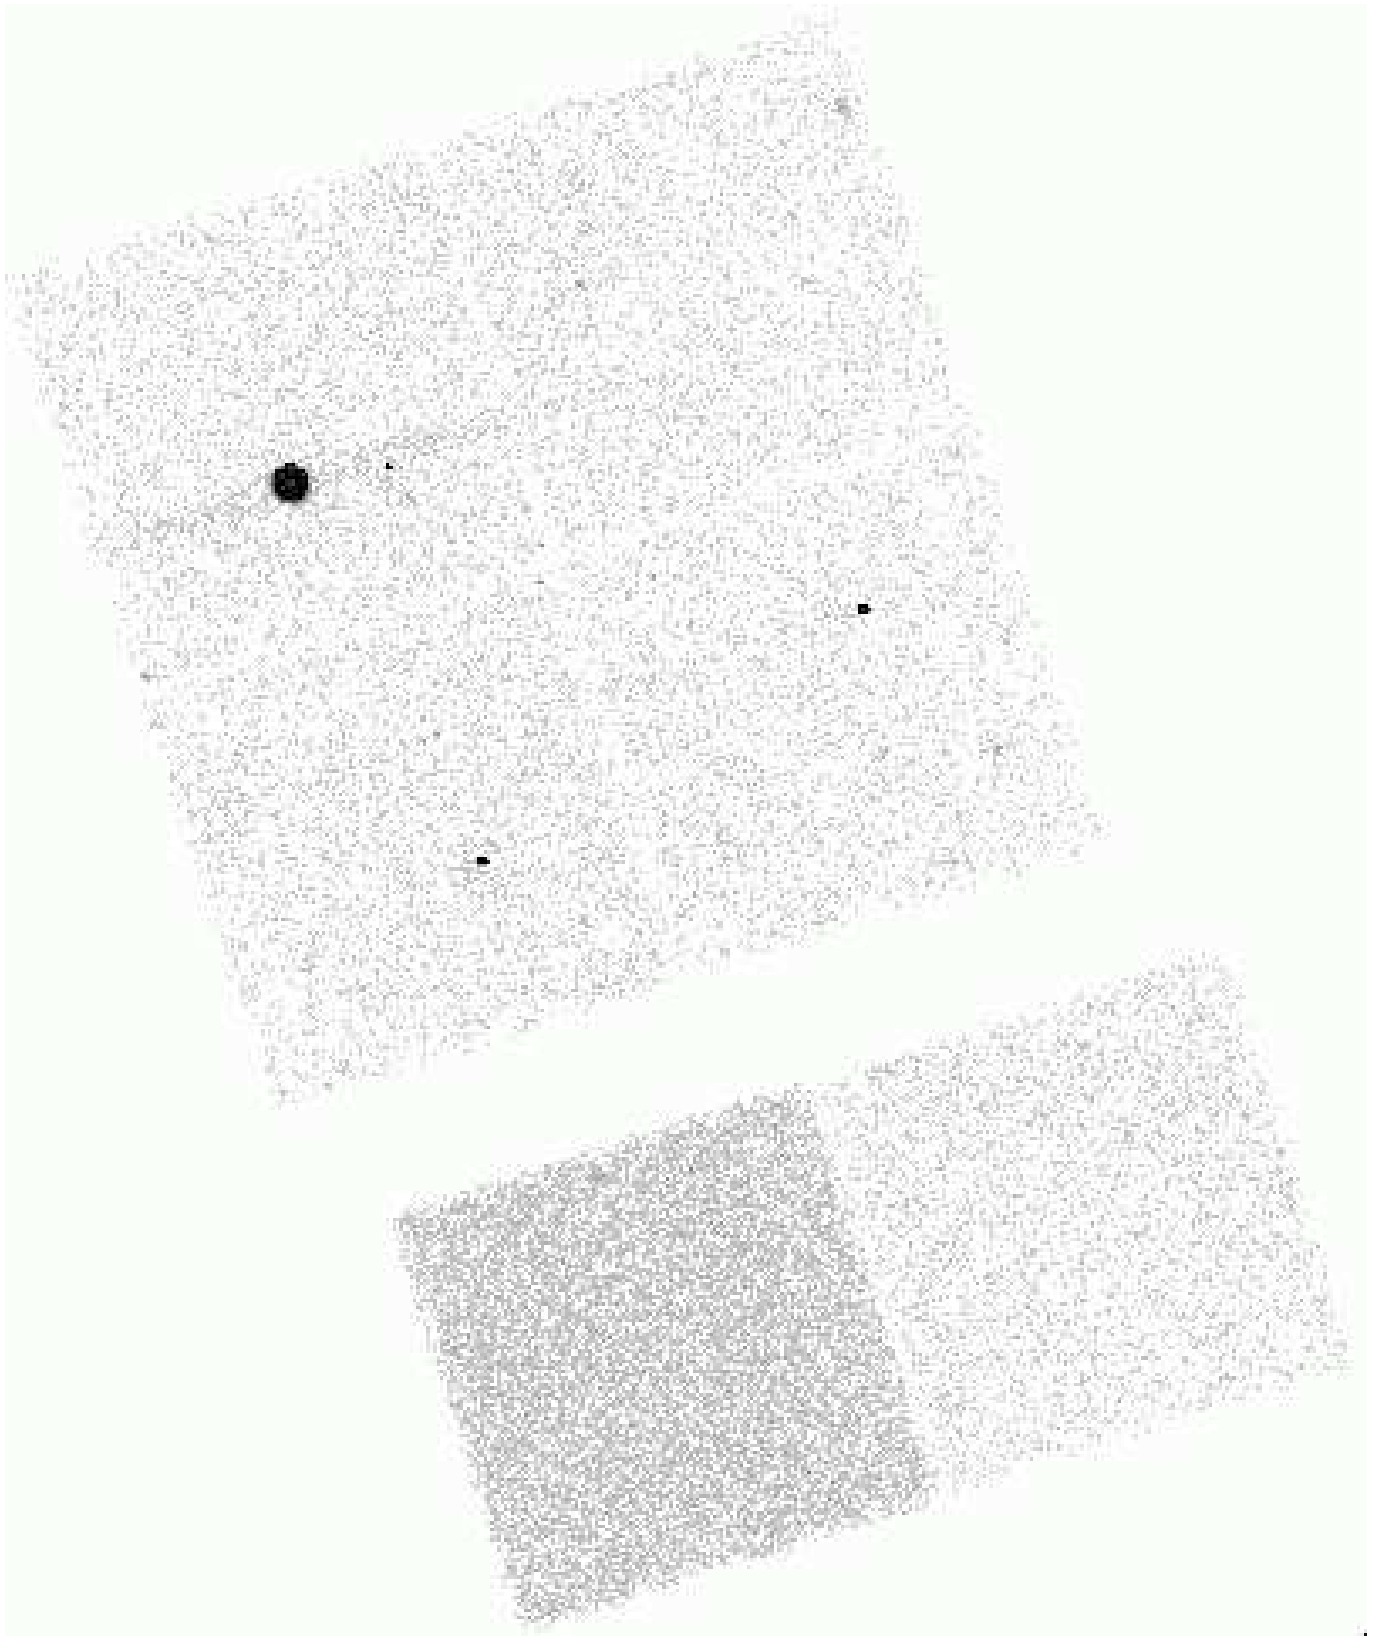

List of the Brighest Sources in the Field

RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
16.018984	-72.033060	932.238647	54.313656	17.163982
15.807756	-72.154040	386.583344	22.725664	17.010872
15.999516	-72.028421	608.333313	49.149307	12.377252
15.406285	-72.072042	185.715912	15.429173	12.036674
16.003668	-72.034547	606.083313	51.350437	11.802885
15.997161	-72.031074	555.750000	49.446907	11.239328
16.007814	-72.027338	550.340881	51.280636	10.731944
16.018662	-72.028943	442.704559	46.739094	9.471826
16.012972	-72.035157	366.041656	43.798038	8.357491
15.906395	-72.025965	89.142860	11.330015	7.867850