Chandra X-ray Center

Seq Num: 590345

Instrument: ACIS

Obs ID: 5147

Source: E0102-72[I3,-120,-4,0.5,0]

PI: Dr. CXC Calibration

Title: AO5A ACIS-I Calibration Observations of E0102-72

---

acisf05147N002 full img2.fits	acisf05147N002 cntr img2.fits
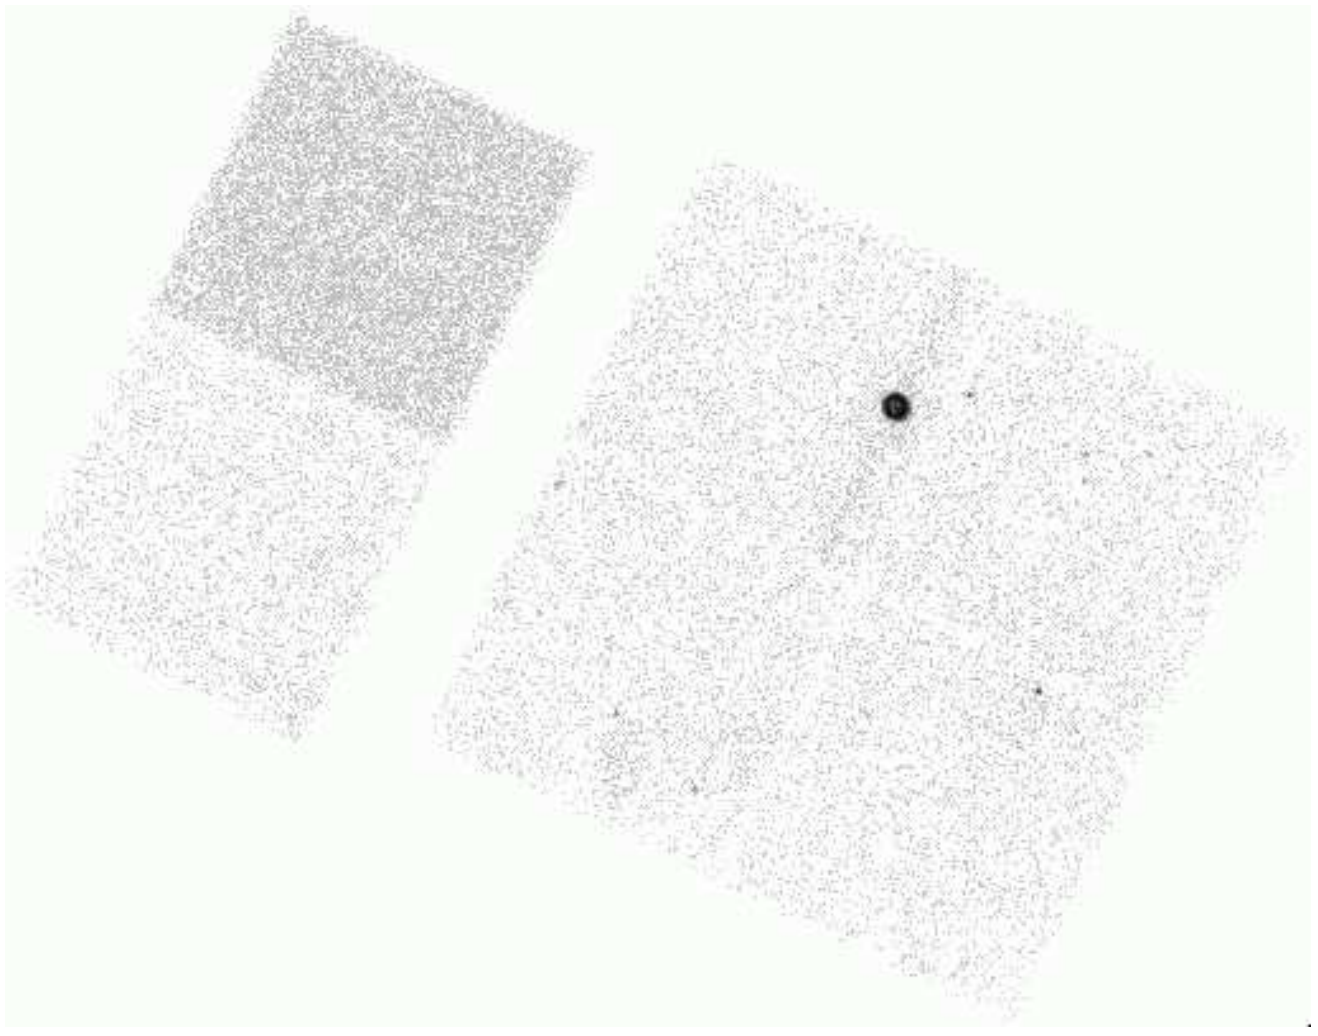	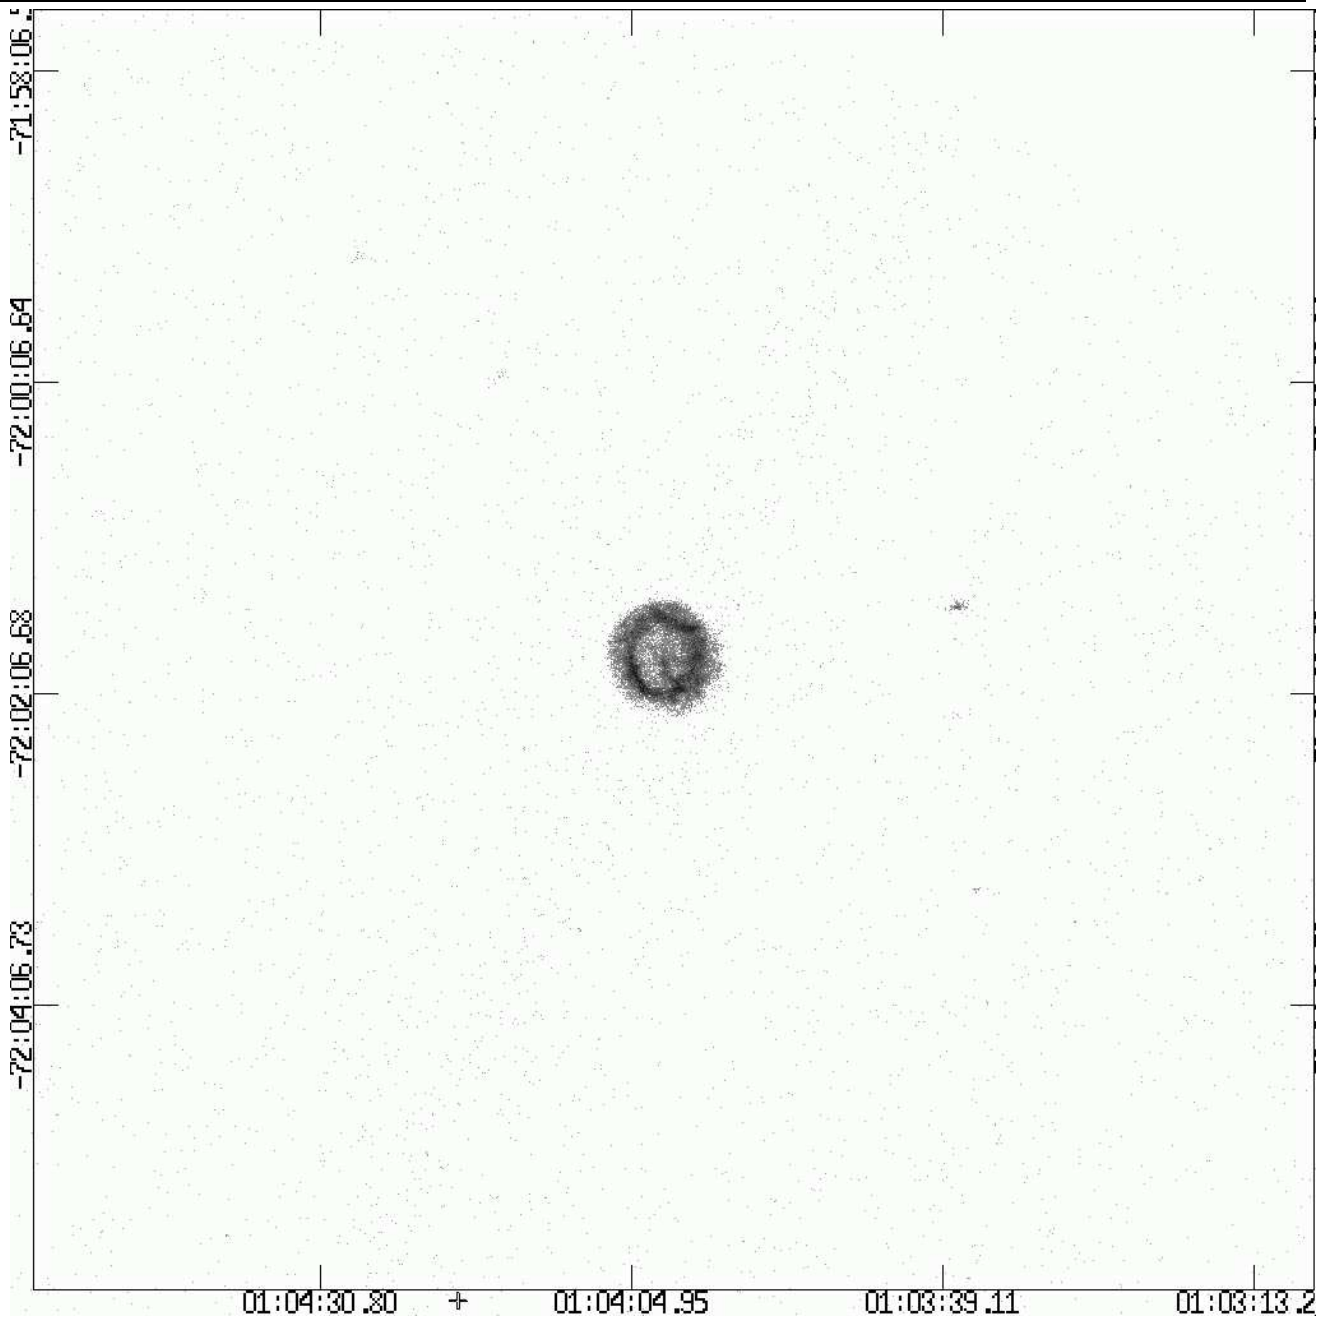

Chandra X-ray Center Seq Num: 590345

Instrument: ACIS Obs ID: 5147

Source: E0102-72[I3,-120,-4,0.5,0] PI: Dr. CXC Calibration

Title: AO5A ACIS-I Calibration Observations of E0102-72

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-06-22T04:21:41	Date and time of file creation
DATE-OBS	2003-12-19T01:58:16	Observation start date
DATE-END	2003-12-19T04:41:27	Observation end date
RA_PNT	16.080430106975	Pointing RA
DEC_PNT	-72.100292957683	Pointing Dec
ROLL_PNT	295.97556558036	Pointing Roll
RA_TARG	16.01	Observer's specified target RA
DEC_TARG	-72.032028	Observer's specified target Dec
DATAMODE	VFAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	153.60722351	Focal Plane Temperature [K]
FSW_VERS	30	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-06-22T04:32:35	Date and time of file creation
DATE-OBS	2003-12-19T01:58:16	Observation start date
DATE-END	2003-12-19T04:41:27	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-012367	Detector
GRATING	NONE	Grating
OBJECT	E0102-72[I3,-120,-4,0.5,0]	Source name
TITLE	AO5A ACIS-I Calibration Observations of E0102-72	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5147	Observation id
SEQ_NUM	590345	Sequence number
RA_NOM	16.080430106975	Nominal RA
DEC_NOM	-72.100292957683	Nominal Dec
ROLL_NOM	295.97556558036	Nominal Roll

Chandra X-ray Center Seq Num: 590345

Instrument: ACIS Obs ID: 5147

Source: E0102-72[I3,-120,-4,0.5,0] PI: Dr. CXC Calibration

Title: AO5A ACIS-I Calibration Observations of E0102-72

Full Field with Sources

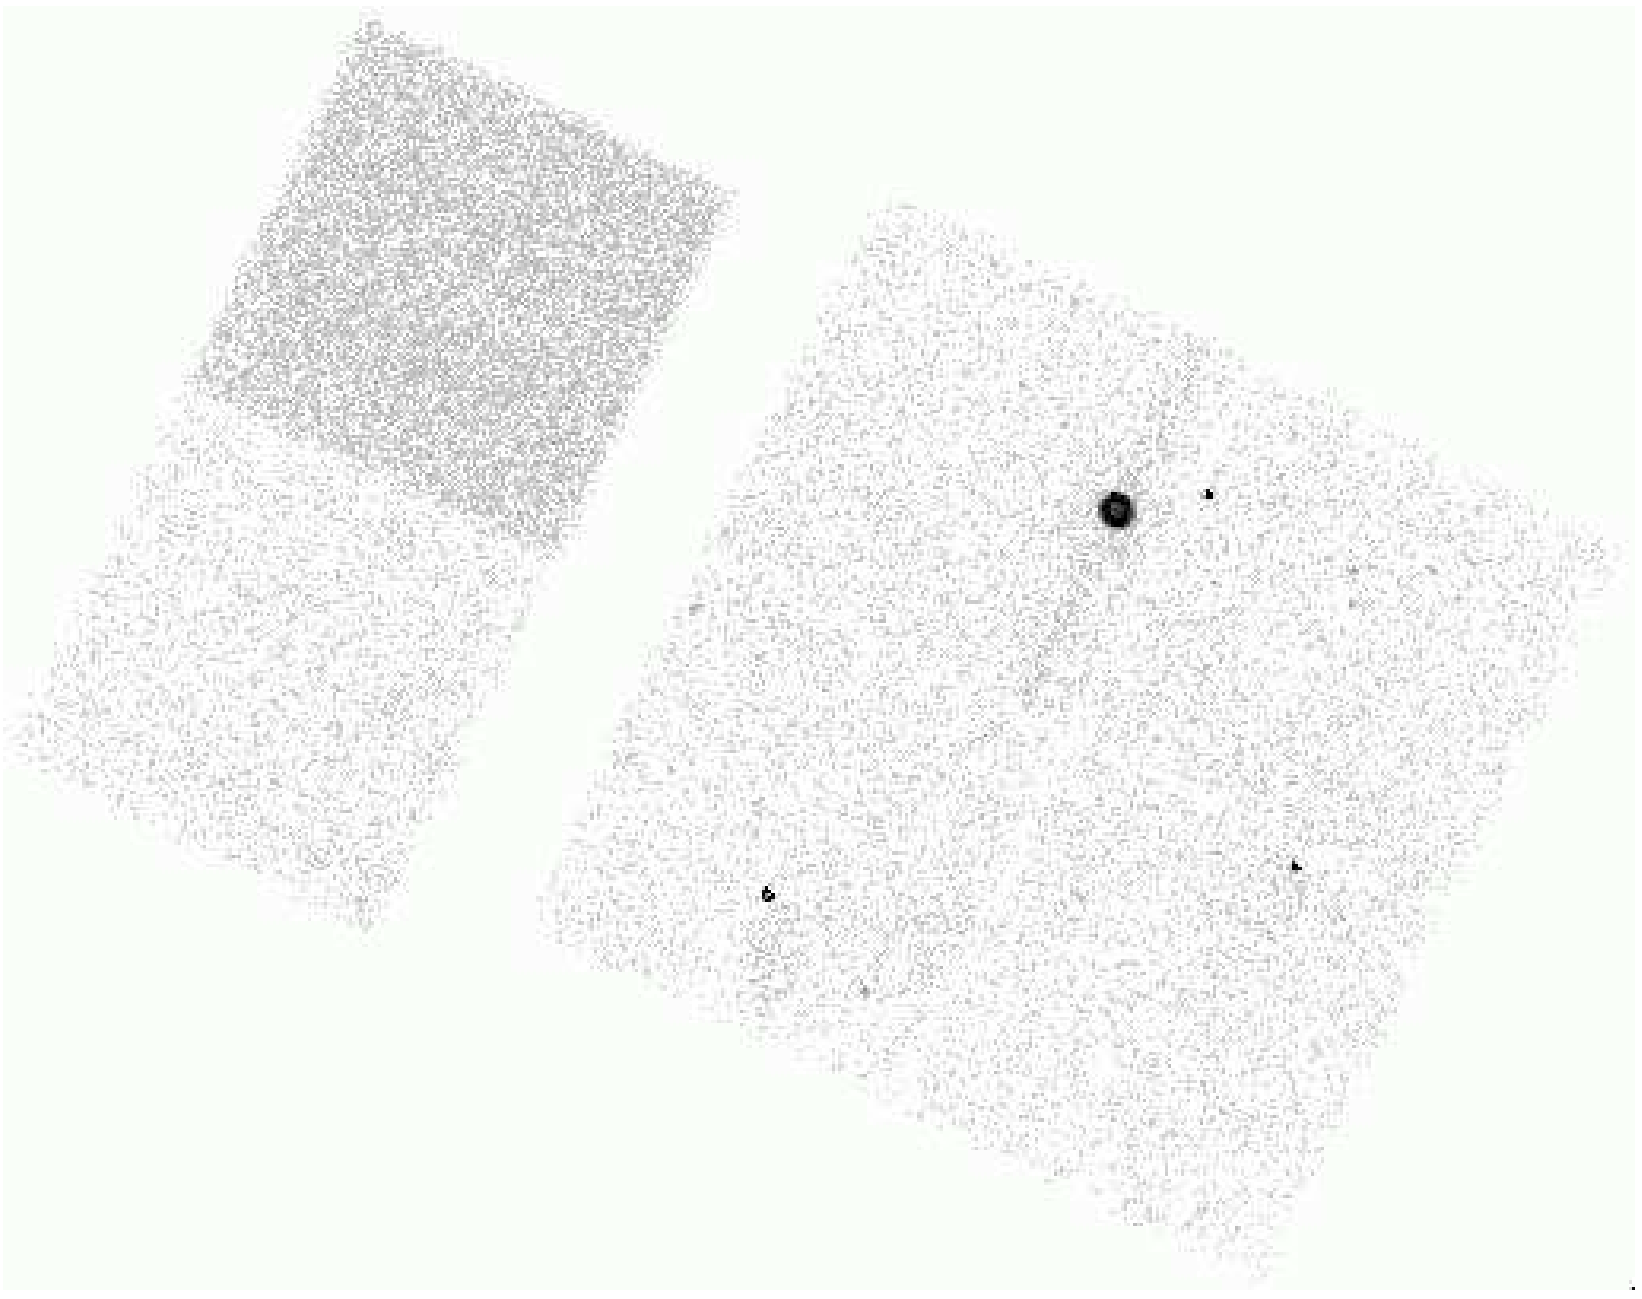

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
15.807973	-72.153956	274.034088	18.449862	14.852907
16.000683	-72.028192	533.857117	49.302540	10.828187
16.019649	-72.033027	520.857117	50.868942	10.239198
16.015243	-72.034707	463.000000	48.652000	9.516566
16.004334	-72.035055	437.285706	48.347923	9.044560
16.009608	-72.027035	394.857147	47.382900	8.333326
16.011397	-72.035205	342.142853	41.700531	8.204761
16.020411	-72.030921	307.714294	40.408897	7.615014
15.906804	-72.025838	92.416664	12.447288	7.424643
16.401704	-72.163397	57.006897	8.966677	6.357639