Chandra X-ray Center

Seq Num: 990002

Instrument: HRC

Obs ID: 5174

Source: RXJ1856.5-3754

PI: Dr. CXC Calibration

Title: AO5 Calibration Observations of the ACIS charged particle background

---

hrcf05174N006 full img2.fits	hrcf05174N006 cntr img2.fits

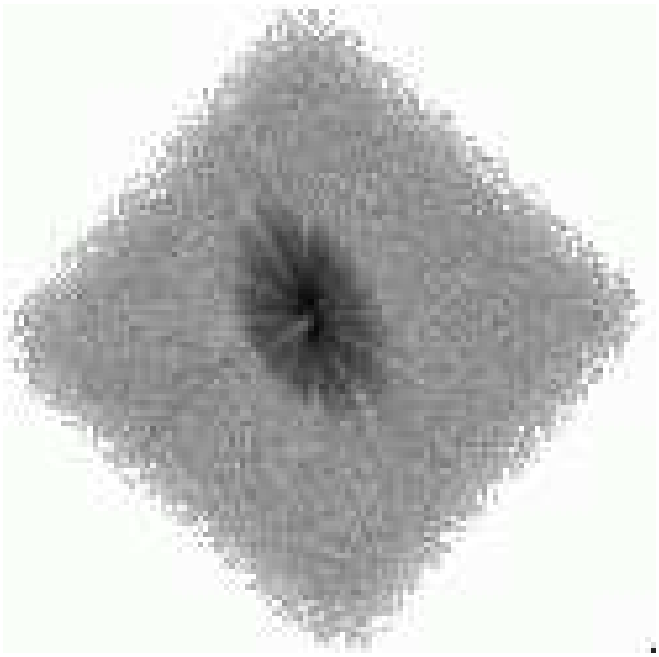

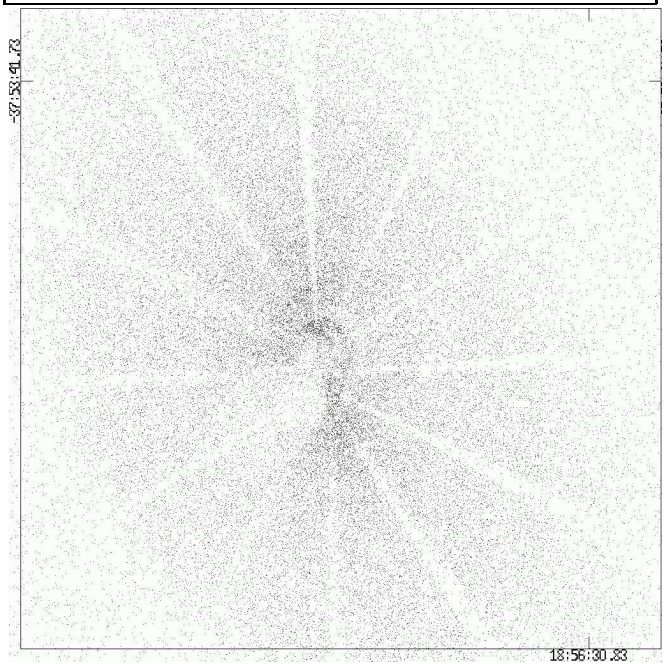

Chandra X-ray Center
Seq Num: 990002
Instrument: HRC
Obs ID: 5174
Source: RXJ1856.5-3754
PI: Dr. CXC Calibration
Title: AO5 Calibration Observations of the ACIS charged particle background

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.10	Processing system revision
DATE	2009-02-09T17:26:47	Date and time of file creation
DATE-OBS	2004-11-04T12:36:41	Observation start date
DATE-END	2004-11-05T02:15:50	Observation end date
RA_PNT	283.67918189652	Pointing RA
DEC_PNT	-37.696391548025	Pointing Dec
ROLL_PNT	266.72891994987	Pointing Roll
RA_TARG	284.147083	Observer's specified target RA
DEC_TARG	-37.909611	Observer's specified target Dec
DEGAP	hrciD1999-07-22gaplookupN0003.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.10	Processing system revision
DATE	2009-02-09T18:15:07	Date and time of file creation
DATE-OBS	2004-11-04T12:36:41	Observation start date
DATE-END	2004-11-05T02:15:50	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-I	Detector
GRATING	NONE	Grating
OBJECT	RXJ1856.5-3754	Source name
TITLE	AO5 Calibration Observations of the ACIS charged particle background	
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5174	Observation id
SEQ_NUM	990002	Sequence number
RA_NOM	283.67918189652	Nominal RA
DEC_NOM	-37.696391548025	Nominal Dec
ROLL_NOM	266.72891994987	Nominal Roll

Chandra X-ray Center
Seq Num: 990002
Instrument: HRC
Obs ID: 5174
Source: RXJ1856.5-3754
PI: Dr. CXC Calibration
Title: AO5 Calibration Observations of the ACIS charged particle background

Full Field with Sources

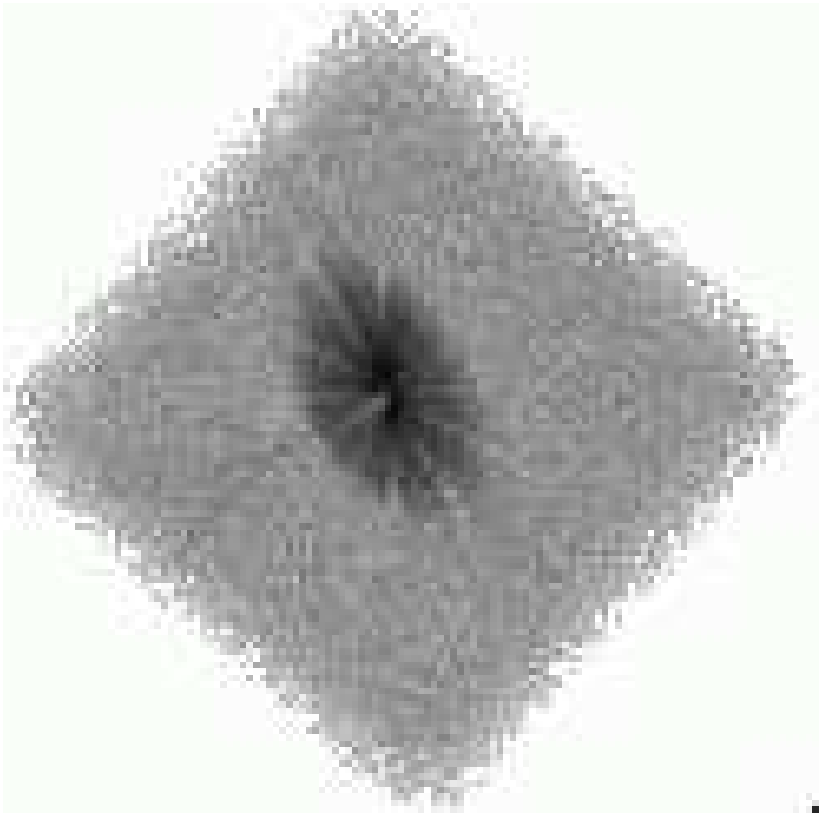

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR