Chandra X-ray Center

Seq Num: 290155

Instrument: HRC

Obs ID: 2599

Source: BETELGEUSE

PI: Dr. CXC Calibration

Title: AO3 CALIBRATION OBSERVATIONS OF BETELGEUSE

---

hrcf02599N002 full img2.fits	hrcf02599N002 cntr img2.fits

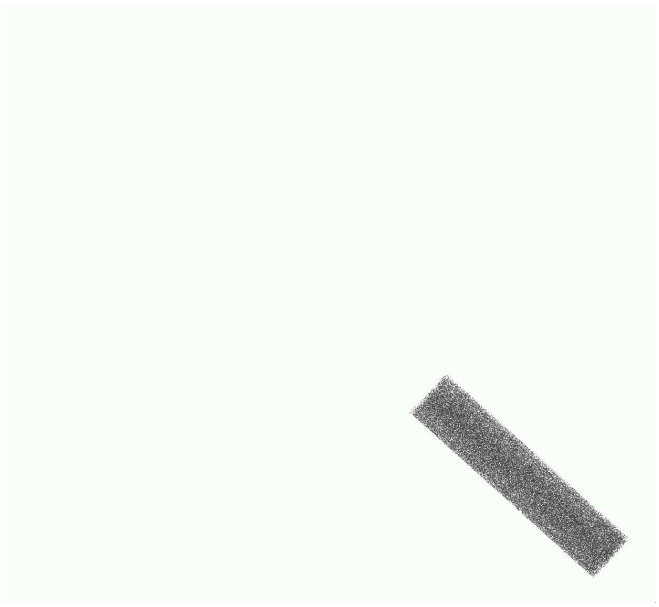

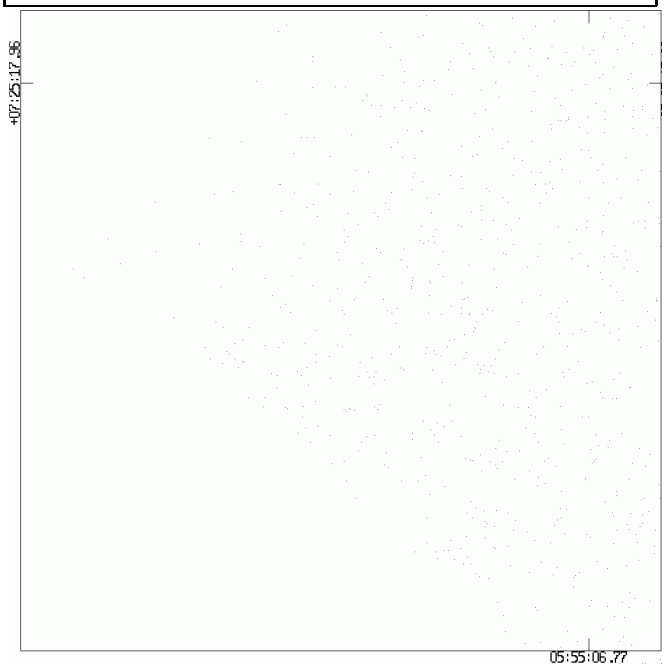

Chandra X-ray Center
Seq Num: 290155
Instrument: HRC
Obs ID: 2599
Source: BETELGEUSE
PI: Dr. CXC Calibration
Title: AO3 CALIBRATION OBSERVATIONS OF BETELGEUSE

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.10	Processing system revision
DATE	2007-01-20T14:06:28	Date and time of file creation
DATE-OBS	2001-12-07T11:08:09	Observation start date
DATE-END	2001-12-07T11:50:35	Observation end date
RA_PNT	89.013093672546	Pointing RA
DEC_PNT	7.6699296068201	Pointing Dec
ROLL_PNT	41.999413756948	Pointing Roll
RA_TARG	88.792917	Observer's specified target RA
DEC_TARG	7.407056	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.10	Processing system revision
DATE	2007-01-20T14:21:40	Date and time of file creation
DATE-OBS	2001-12-07T11:08:09	Observation start date
DATE-END	2001-12-07T11:50:35	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	NONE	Grating
OBJECT	BETELGEUSE	Source name
TITLE	AO3 CALIBRATION OBSERVATIONS OF BETELGEUSE	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	2599	Observation id
SEQ_NUM	290155	Sequence number
RA_NOM	89.013093672546	Nominal RA
DEC_NOM	7.6699296068201	Nominal Dec
ROLL_NOM	41.999413756948	Nominal Roll

Chandra X-ray Center
Seq Num: 290155
Instrument: HRC
Obs ID: 2599
Source: BETELGEUSE
PI: Dr. CXC Calibration
Title: AO3 CALIBRATION OBSERVATIONS OF BETELGEUSE

Full Field with Sources

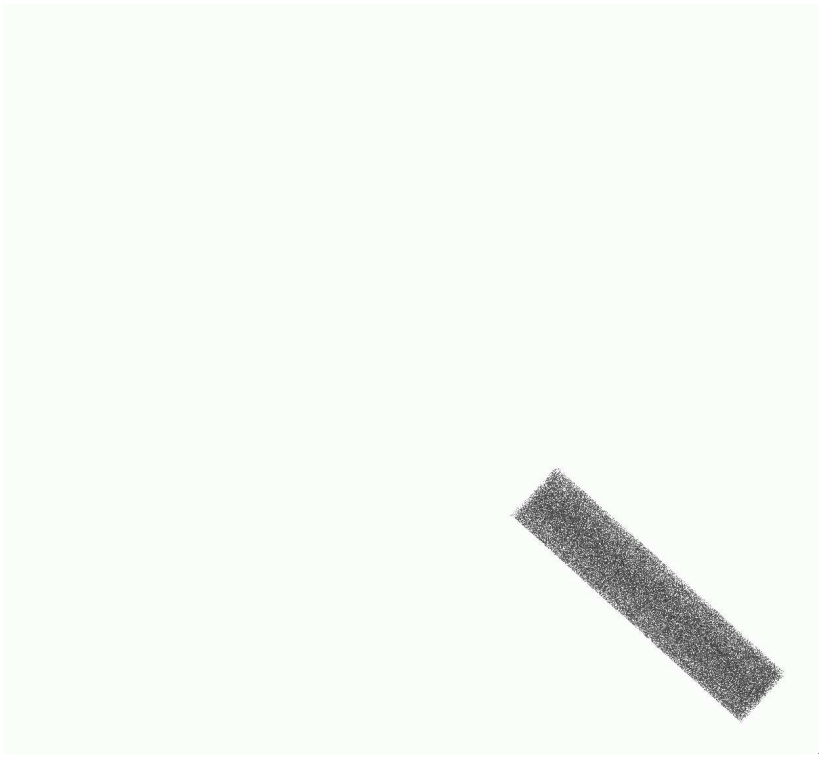

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR