Summary Page Created:Thu August 31, 2006 07:09 EDT

Chandra X-ray Center

Seq Num: 590259

Instrument: ACIS

Obs ID: 2870

Source: CAS A [Chip S3, T=120, Offsets=-2,0,0]

PI: Dr. CXC Calibration

Title: AO3A CALIBRATION OBSERVATIONS THE STANDARD CANDLES CAS A AND G21.5-09

---

acisf02870N002 full img2.fits	acisf02870N002 cntr img2.fits

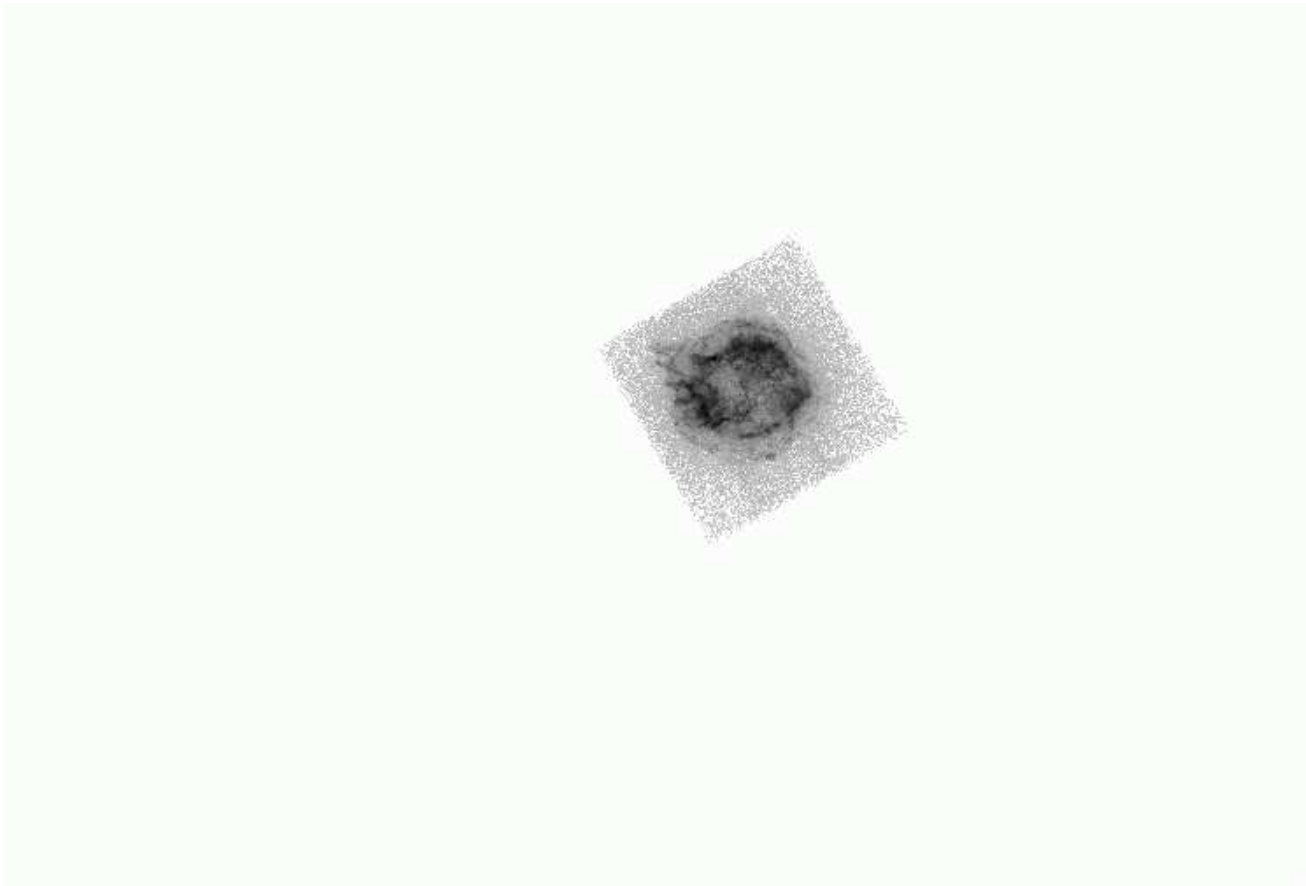

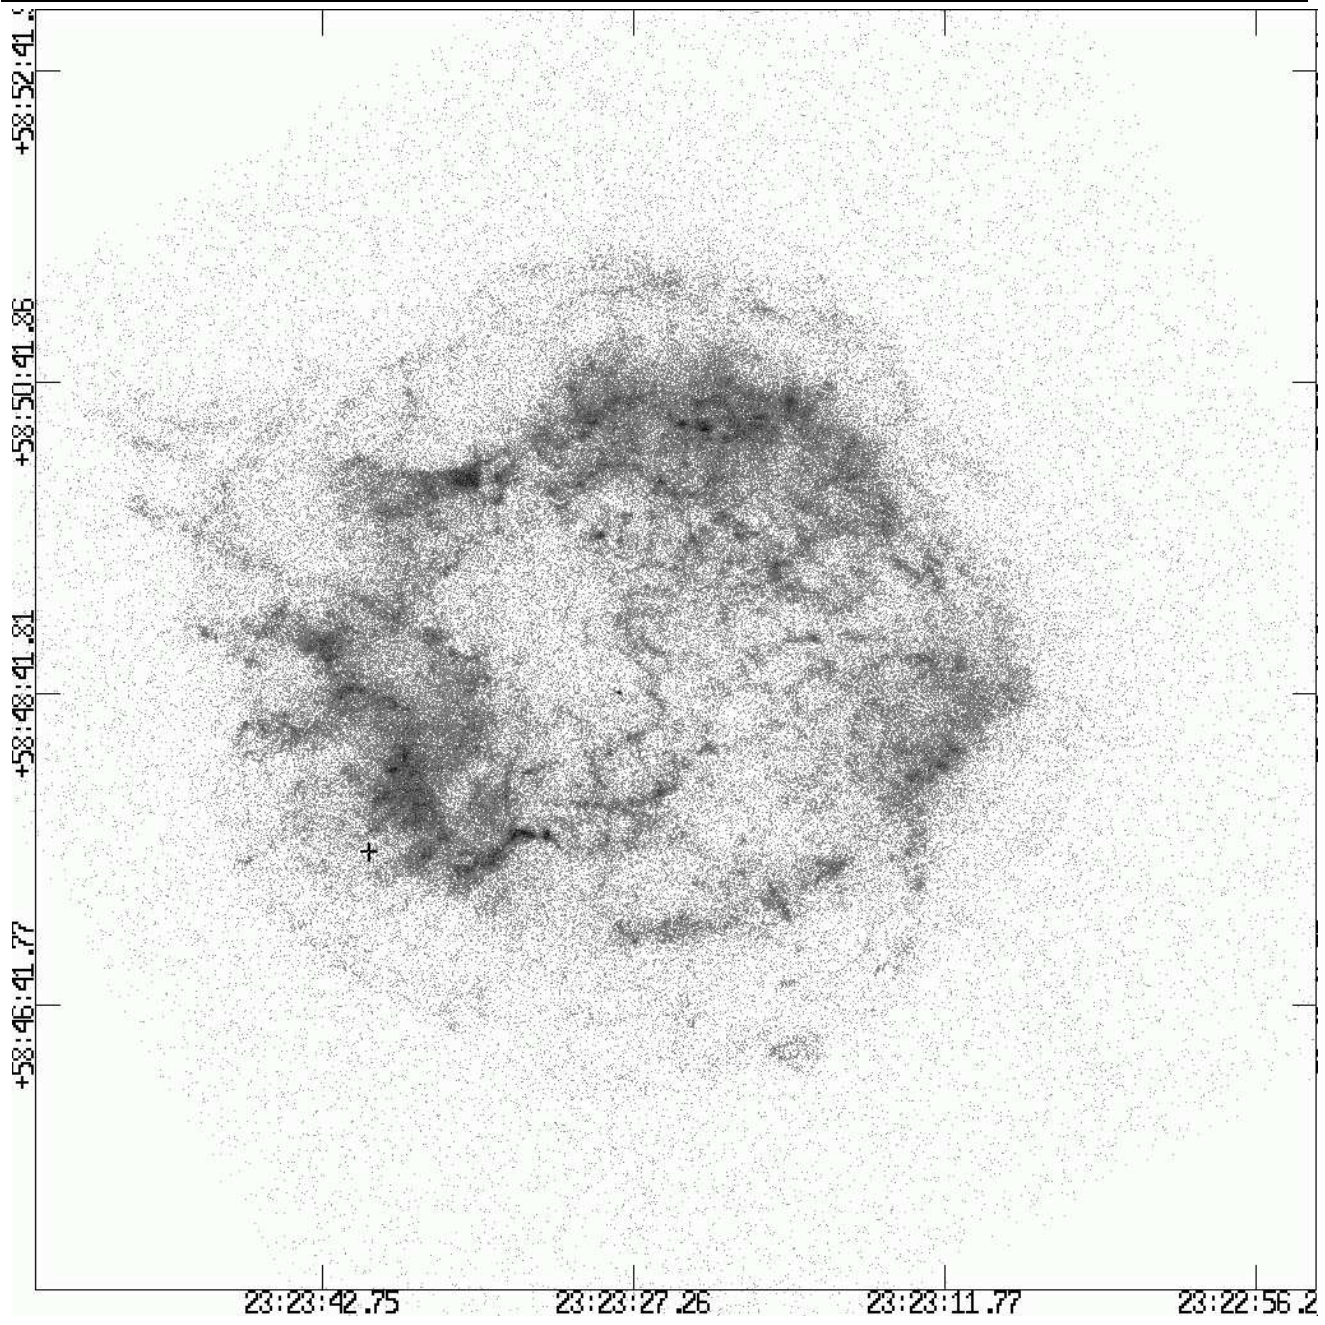

Chandra X-ray Center Seq Num: 590259

Instrument: ACIS Obs ID: 2870

Source: CAS A [Chip S3, T=120, Offsets=-2,0,0] PI: Dr. CXC Calibration

Title: AO3A CALIBRATION OBSERVATIONS THE STANDARD CANDLES CAS A AND G21.5-09

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8.1	ASCDS version number
DATE	2006-08-31T10:47:35	Date and time of file creation
DATE-OBS	2002-02-06T20:39:48	Observation start date
DATE-END	2002-02-06T21:38:43	Observation end date
RA_PNT	350.91836514445	Pointing RA
DEC_PNT	58.794643012511	Pointing Dec
ROLL_PNT	330.13289460444	Pointing Roll
RA_TARG	350.8575	Observer's specified target RA
DEC_TARG	58.814833	Observer's specified target Dec
DATAMODE	FAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	153.4460144	Focal Plane Temperature [K]
FSW_VERS	30	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8.1	ASCDS version number
DATE	2006-08-31T11:07:41	Date and time of file creation
DATE-OBS	2002-02-06T20:39:48	Observation start date
DATE-END	2002-02-06T21:38:43	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-456789	Detector
GRATING	NONE	Grating
OBJECT	CAS A [Chip S3, T=120, Offsets=-2,0,0]	Source name
TITLE	AO3A CALIBRATION OBSERVATIONS THE STANDARD CANDLES CAS A AND G21.5-09	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	2870	Observation id
SEQ_NUM	590259	Sequence number
RA_NOM	350.91836514445	Nominal RA
DEC_NOM	58.794643012511	Nominal Dec
ROLL_NOM	330.13289460444	Nominal Roll

Chandra X-ray Center

Seq Num: 590259

Instrument: ACIS

Obs ID: 2870

Source: CAS A [Chip S3, T=120, Offsets=-2,0,0]

PI: Dr. CXC Calibration

Title: AO3A CALIBRATION OBSERVATIONS THE STANDARD CANDLES CAS A AND G21.5-09

Full Field with Sources

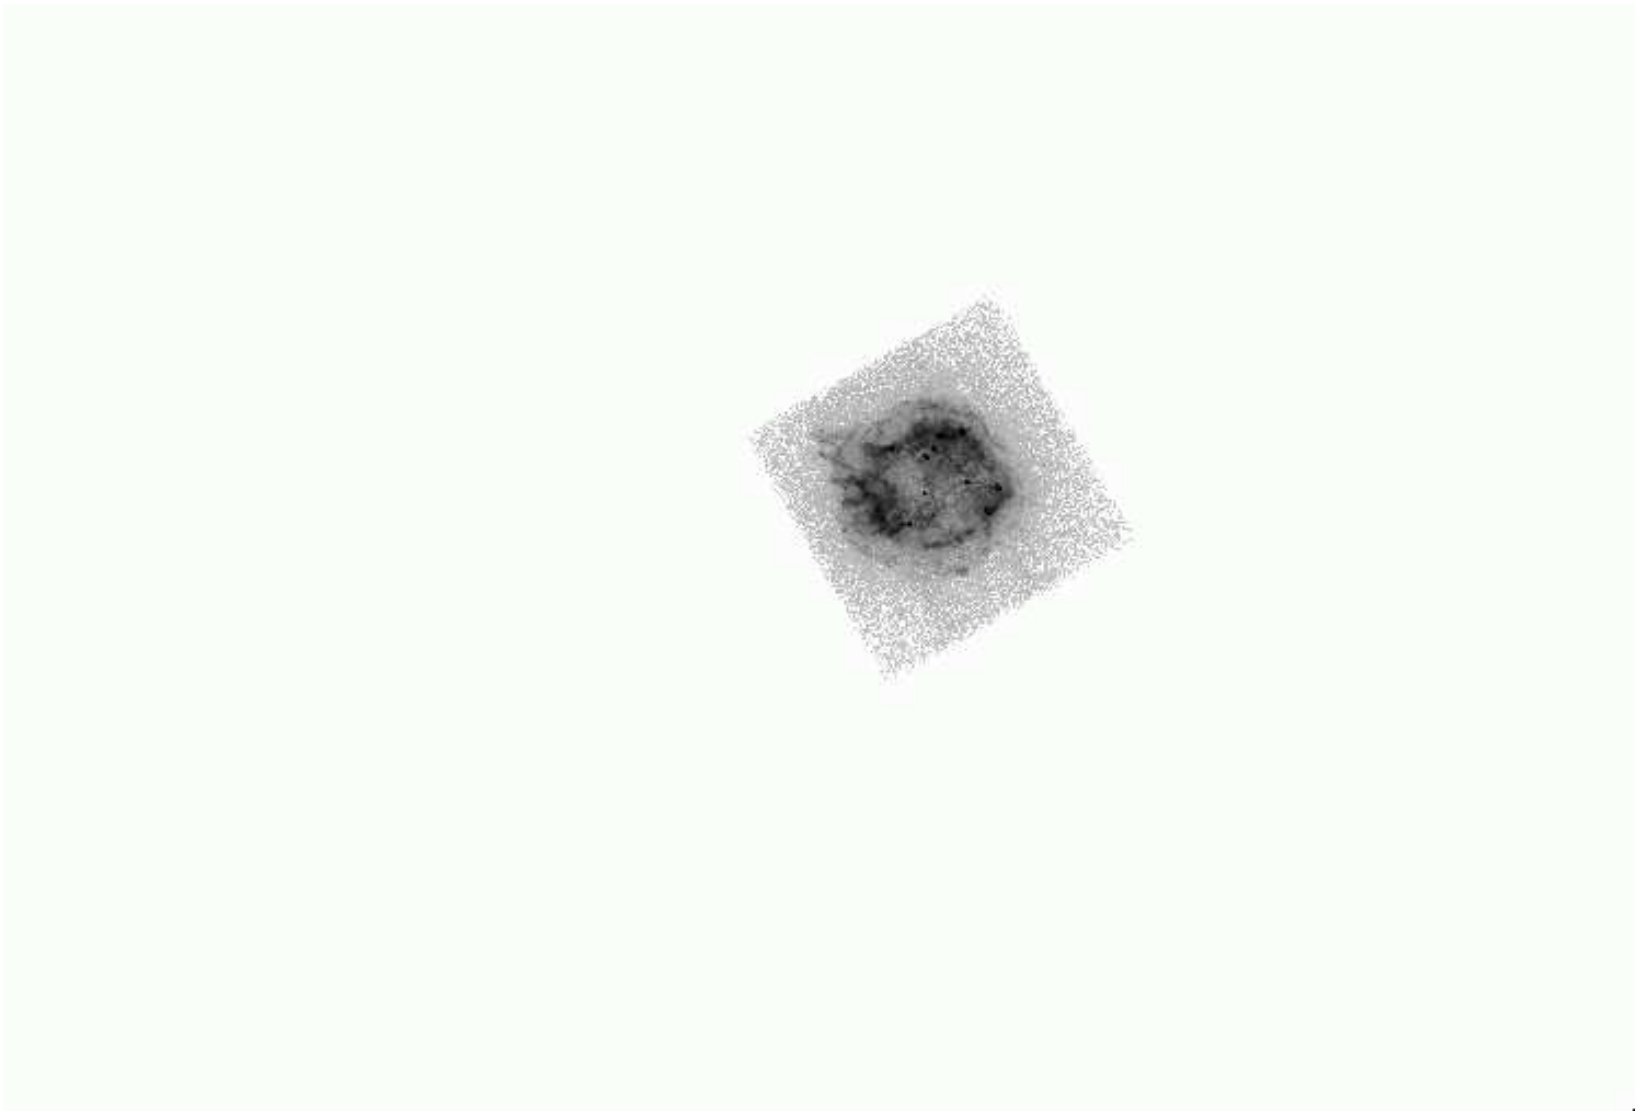

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
350.848588	58.840161	346.920441	34.878922	9.946422
350.853306	58.840558	232.056824	29.460979	7.876751
350.858012	58.834396	172.272720	23.996468	7.179087
350.830801	58.842703	290.714294	40.983368	7.093470
350.881436	58.796531	168.714279	25.347664	6.656009
350.826280	58.817594	117.761360	17.748024	6.635182
350.866499	58.811760	85.428574	13.087655	6.527416
350.795953	58.814766	178.571426	27.447758	6.505866
350.865018	58.830422	110.681816	17.477903	6.332672
350.805400	58.802764	201.285721	32.611656	6.172202