Chandra X-ray Center
Seq Num: 290237
Instrument: HRC
Obs ID: 3683
Source: BETELGEUSE
PI: Dr. CXC Calibration
Title: AO4 MEASUREMENTS OF THE OPTICAL/UV TRANSMISSION OF THE HRC AND ACIS FILTERS

---

hrcf03683N002 full img2.fits

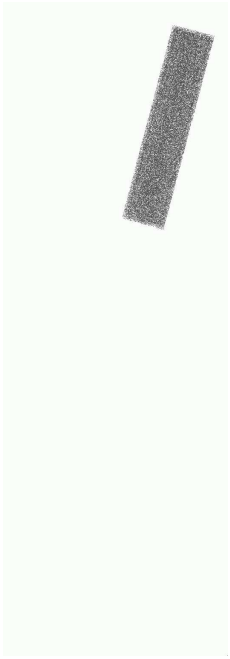

hrcf03683N002 cntr img2.fits

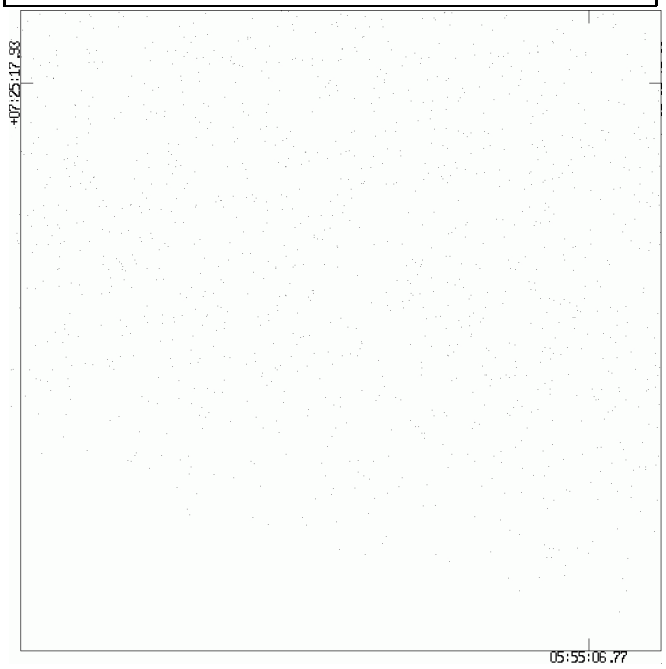

Chandra X-ray Center
Seq Num: 290237
Instrument: HRC
Obs ID: 3683
Source: BETELGEUSE
PI: Dr. CXC Calibration
Title: AO4 MEASUREMENTS OF THE OPTICAL/UV TRANSMISSION OF THE HRC AND ACIS FILTERS

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	Processing system revision
DATE	2006-07-20T19:50:25	Date and time of file creation
DATE-OBS	2003-02-06T04:50:43	Observation start date
DATE-END	2003-02-06T05:32:33	Observation end date
RA_PNT	88.878929630062	Pointing RA
DEC_PNT	7.0799986561218	Pointing Dec
ROLL_PNT	284.71332590419	Pointing Roll
RA_TARG	88.792917	Observer's specified target RA
DEC_TARG	7.407056	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	Processing system revision
DATE	2006-07-20T20:06:46	Date and time of file creation
DATE-OBS	2003-02-06T04:50:43	Observation start date
DATE-END	2003-02-06T05:32:33	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	NONE	Grating
OBJECT	BETELGEUSE	Source name
TITLE	AO4 MEASUREMENTS OF THE OPTICAL/UV TRANSMISSION OF THE HRC AND ACIS FILTERS	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	3683	Observation id
SEQ_NUM	290237	Sequence number
RA_NOM	88.878929630062	Nominal RA
DEC_NOM	7.0799986561218	Nominal Dec
ROLL_NOM	284.71332590419	Nominal Roll

Chandra X-ray Center
Seq Num: 290237
Instrument: HRC
Obs ID: 3683
Source: BETELGEUSE
PI: Dr. CXC Calibration
Title: AO4 MEASUREMENTS OF THE OPTICAL/UV TRANSMISSION OF THE HRC AND ACIS FILTERS

Full Field with Sources

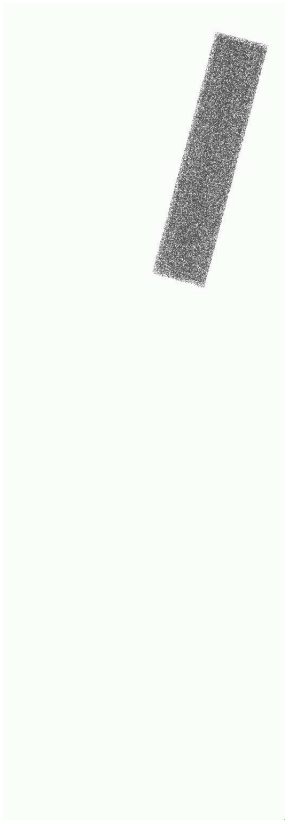

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR