Chandra X-ray Center

Instrument: HRC
Source: HZ43
Grating: LETG
Title: AO5 Calibration Observations of HZ43

Seq Num: 290315
Obs ID: 5042
PI: Dr. CXC Calibration

hrcf05042N002 full img2.fits	hrcf05042N002 cntr img2.fits
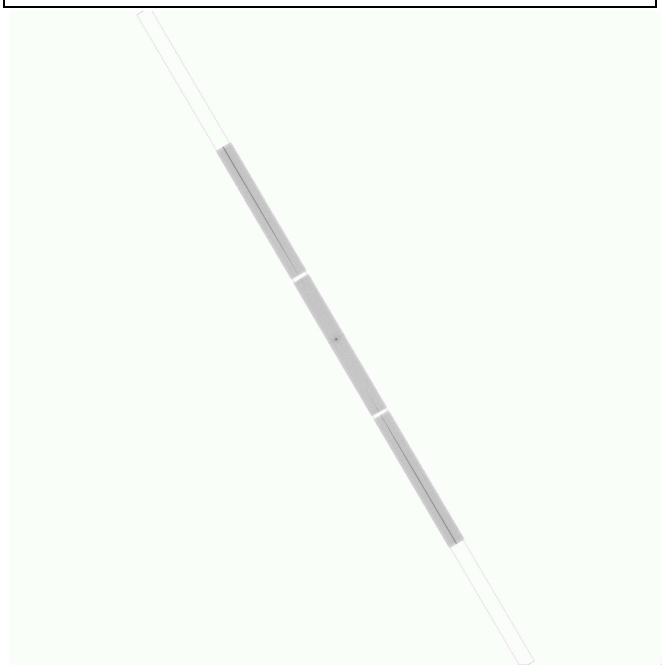	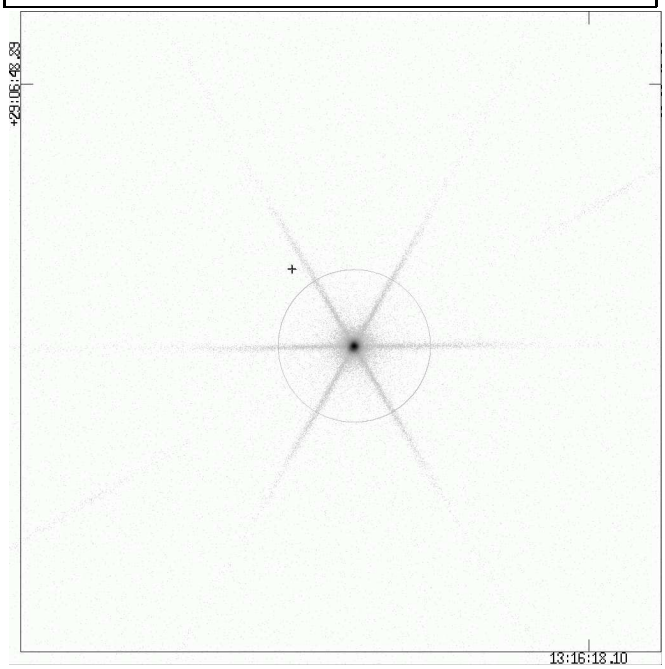

Chandra X-ray Center
Seq Num: 290315
Instrument: HRC
Obs ID: 5042
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO5 Calibration Observations of HZ43

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-06-22T06:43:45	Date and time of file creation
DATE-OBS	2003-12-20T15:02:58	Observation start date
DATE-END	2003-12-20T21:09:28	Observation end date
RA_PNT	199.0948808891	Pointing RA
DEC_PNT	29.102958628924	Pointing Dec
ROLL_PNT	59.420021603054	Pointing Roll
RA_TARG	199.092083	Observer's specified target RA
DEC_TARG	29.099	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-06-22T07:02:47	Date and time of file creation
DATE-OBS	2003-12-20T15:02:58	Observation start date
DATE-END	2003-12-20T21:09:28	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	LETG	Grating
OBJECT	HZ43	Source name
TITLE	AO5 Calibration Observations of HZ43	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5042	Observation id
SEQ_NUM	290315	Sequence number
RA_NOM	199.0948808891	Nominal RA
DEC_NOM	29.102958628924	Nominal Dec
ROLL_NOM	59.420021603054	Nominal Roll

Chandra X-ray Center
Seq Num: 290315
Instrument: HRC
Obs ID: 5042
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO5 Calibration Observations of HZ43
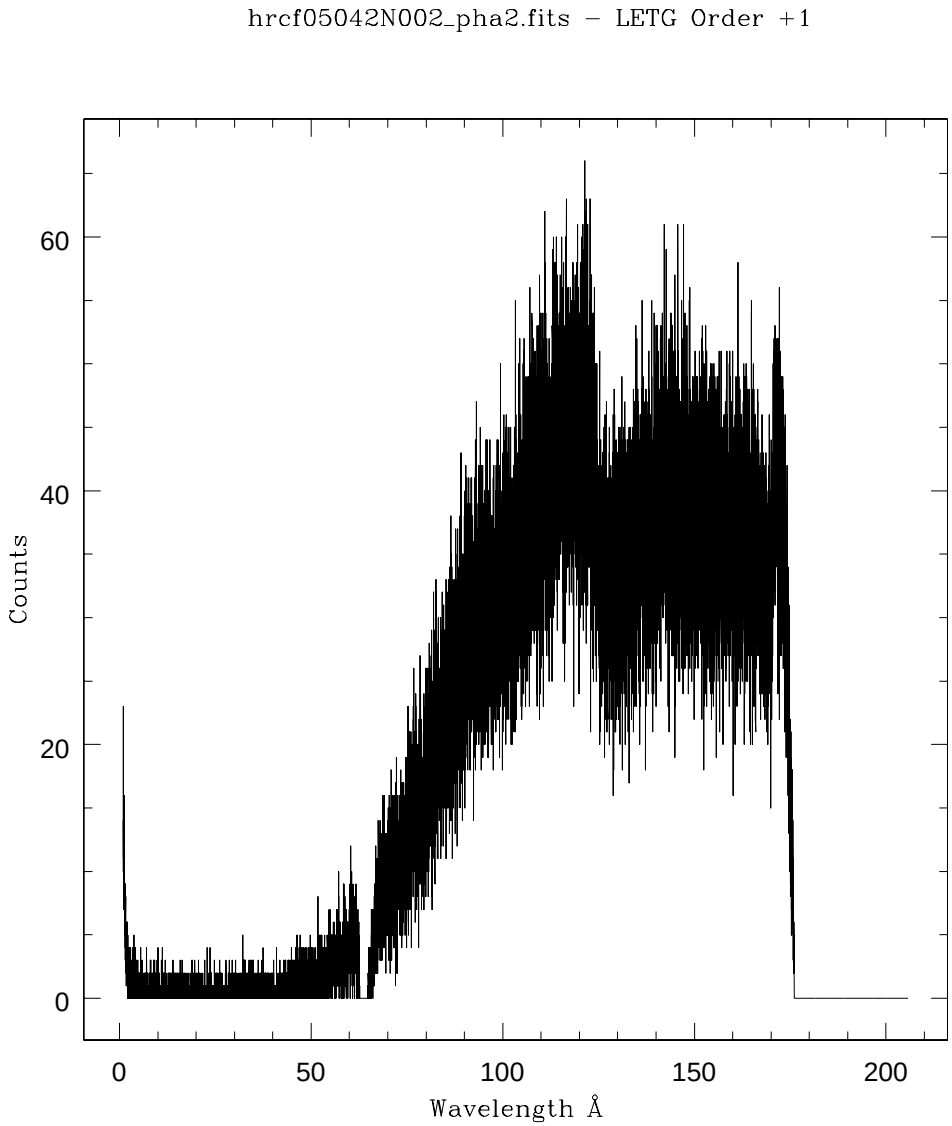
LETG +1 order