Chandra X-ray Center

Instrument: HRC
Source: HZ43
Grating: LETG
Title: AO5 Calibration Observations of HZ43

Seq Num: 290317
Obs ID: 5044
PI: Dr. CXC Calibration

hrcf05044N002 full img2.fits	hrcf05044N002 cntr img2.fits
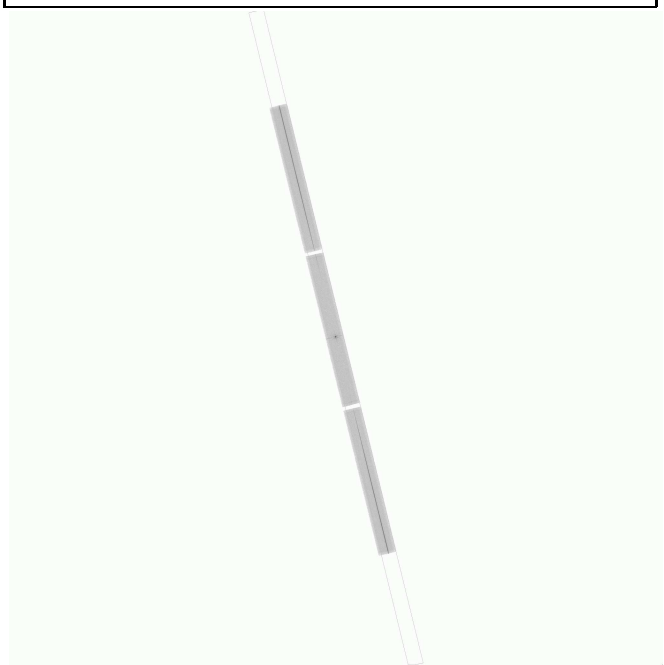	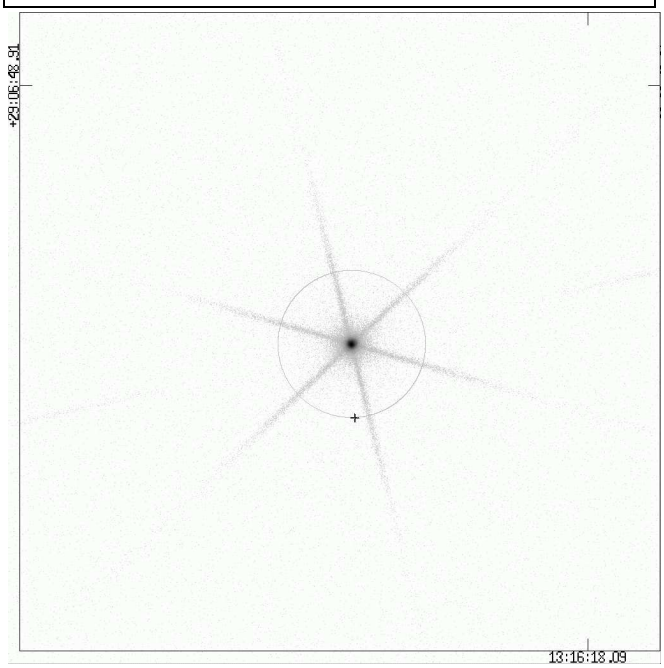

Chandra X-ray Center
Seq Num: 290317
Instrument: HRC
Obs ID: 5044
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO5 Calibration Observations of HZ43

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.2	ASCDS version number
DATE	2006-04-28T04:42:16	Date and time of file creation
DATE-OBS	2004-07-19T17:11:43	Observation start date
DATE-END	2004-07-19T23:00:04	Observation end date
RA_PNT	199.09064960052	Pointing RA
DEC_PNT	29.094448431665	Pointing Dec
ROLL_PNT	256.19410795692	Pointing Roll
RA_TARG	199.092083	Observer's specified target RA
DEC_TARG	29.099	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.2	ASCDS version number
DATE	2006-04-28T05:04:44	Date and time of file creation
DATE-OBS	2004-07-19T17:11:43	Observation start date
DATE-END	2004-07-19T23:00:04	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	LETG	Grating
OBJECT	HZ43	Source name
TITLE	AO5 Calibration Observations of HZ43	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5044	Observation id
SEQ_NUM	290317	Sequence number
RA_NOM	199.09064960052	Nominal RA
DEC_NOM	29.094448431665	Nominal Dec
ROLL_NOM	256.19410795692	Nominal Roll

Chandra X-ray Center
Seq Num: 290317
Instrument: HRC
Obs ID: 5044
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO5 Calibration Observations of HZ43
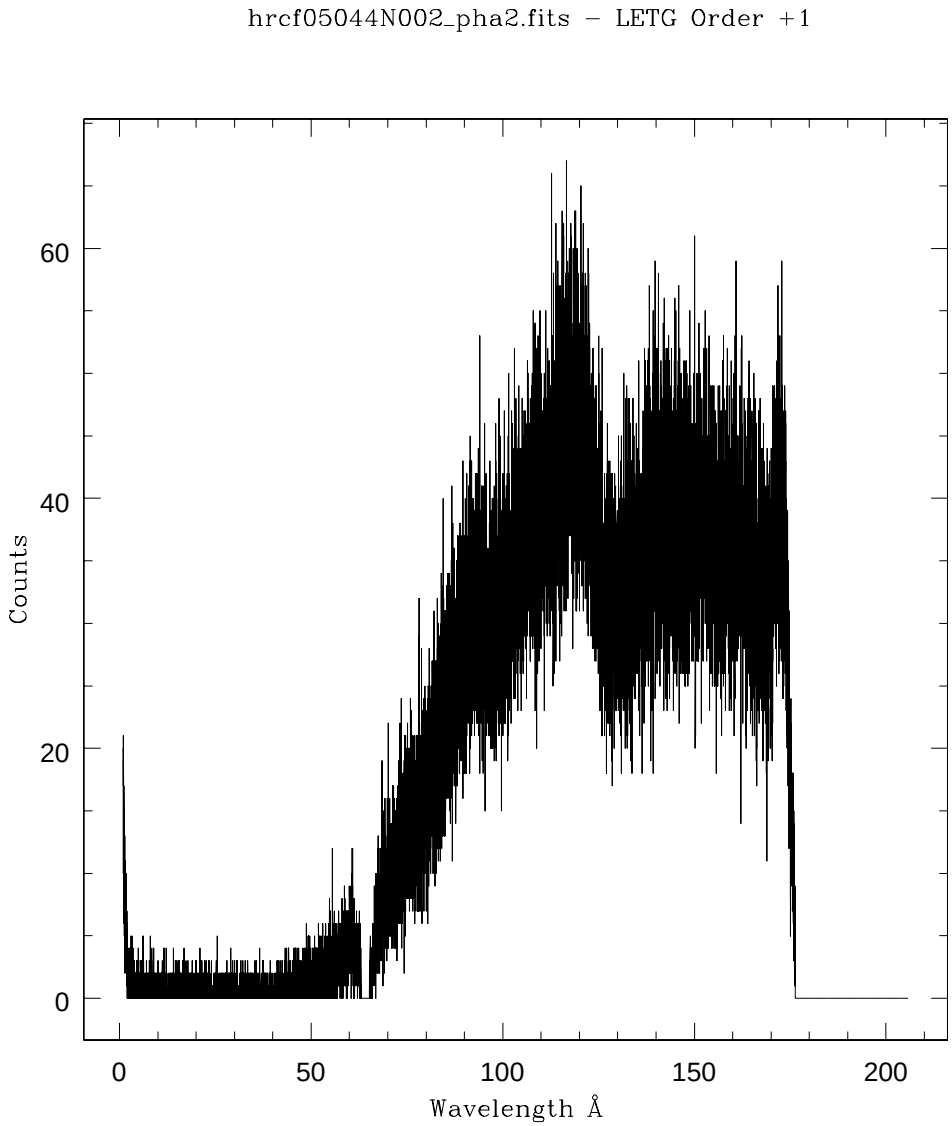
LETG +1 order