Chandra X-ray Center

Instrument: HRC
Source: HZ43
Grating: LETG
Title: AO5 Calibration Observations of HZ43

Seq Num: 290318
Obs ID: 5045
PI: Dr. CXC Calibration

hrcf05045N003 full img2.fits	hrcf05045N003 cntr img2.fits

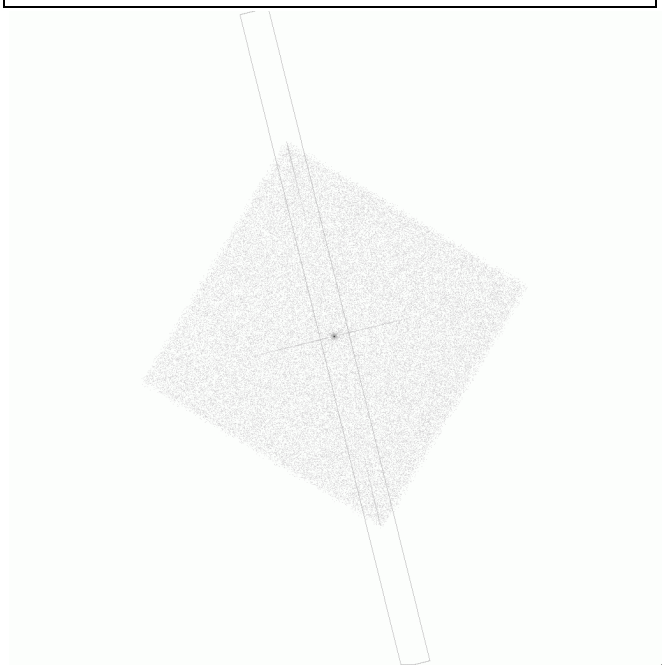

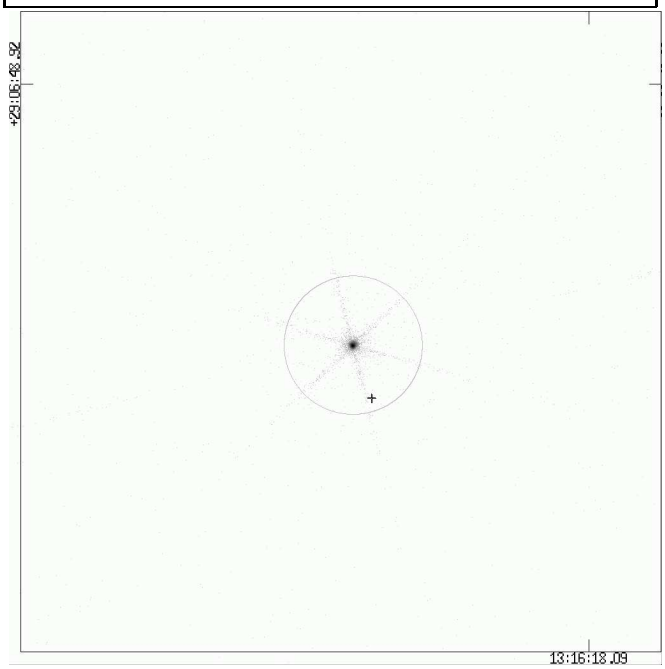

Chandra X-ray Center
Seq Num: 290318
Instrument: HRC
Obs ID: 5045
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO5 Calibration Observations of HZ43

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.2	ASCDS version number
DATE	2007-11-24T00:24:15	Date and time of file creation
DATE-OBS	2004-07-19T16:17:33	Observation start date
DATE-END	2004-07-19T17:11:43	Observation end date
RA_PNT	199.08961831626	Pointing RA
DEC_PNT	29.095567074277	Pointing Dec
ROLL_PNT	256.00368010778	Pointing Roll
RA_TARG	199.092083	Observer's specified target RA
DEC_TARG	29.099	Observer's specified target Dec
DEGAP	hrciD1999-07-22gaplookupN0003.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.2	ASCDS version number
DATE	2007-11-24T00:34:37	Date and time of file creation
DATE-OBS	2004-07-19T16:17:33	Observation start date
DATE-END	2004-07-19T17:11:43	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-I	Detector
GRATING	LETG	Grating
OBJECT	HZ43	Source name
TITLE	AO5 Calibration Observations of HZ43	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5045	Observation id
SEQ_NUM	290318	Sequence number
RA_NOM	199.08961831626	Nominal RA
DEC_NOM	29.095567074277	Nominal Dec
ROLL_NOM	256.00368010778	Nominal Roll

Chandra X-ray Center
Seq Num: 290318
Instrument: HRC
Obs ID: 5045
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO5 Calibration Observations of HZ43
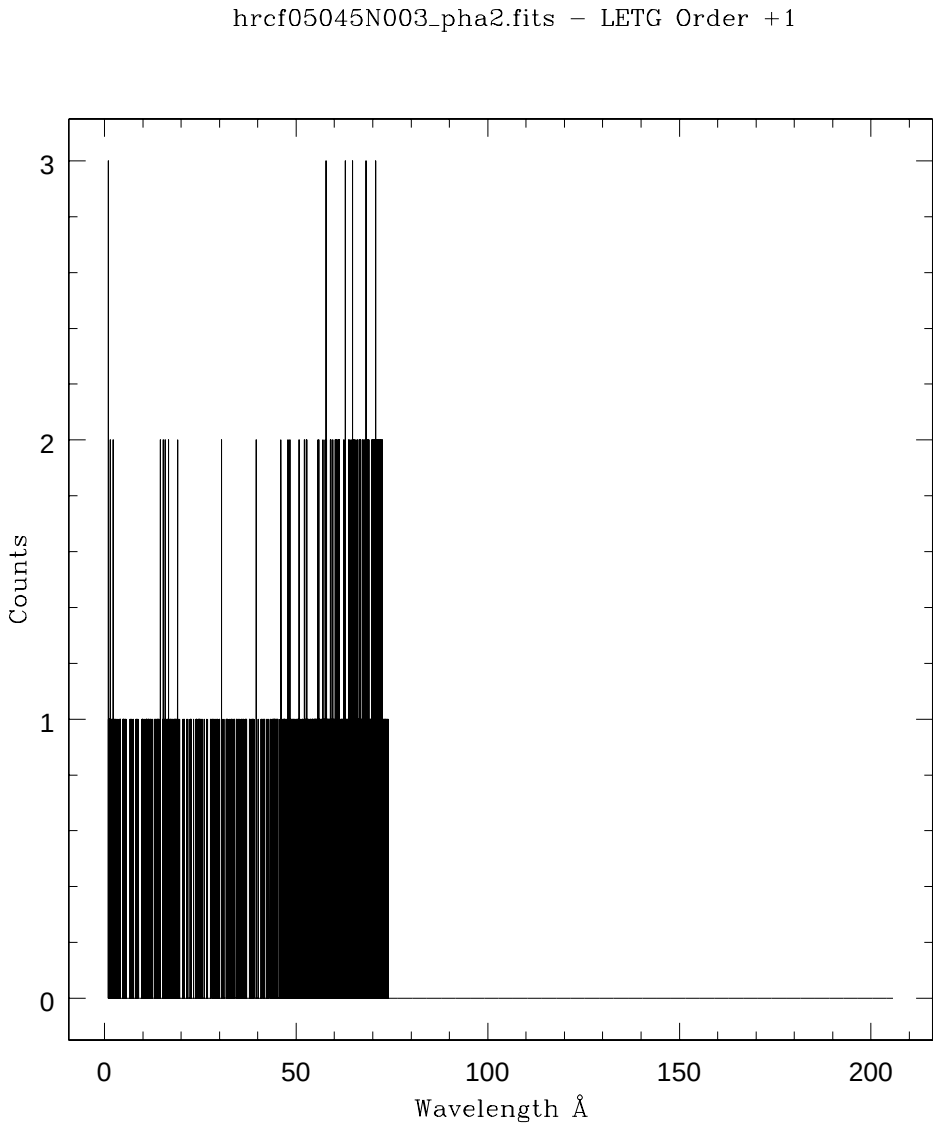
LETG +1 order