Chandra X-ray Center

Seq Num: 290326

Instrument: HRC

Obs ID: 5053

Source: Vega

PI: Dr. CXC Calibration

Title: AO5 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

---

hrcf05053N002 full img2.fits	hrcf05053N002 cntr img2.fits

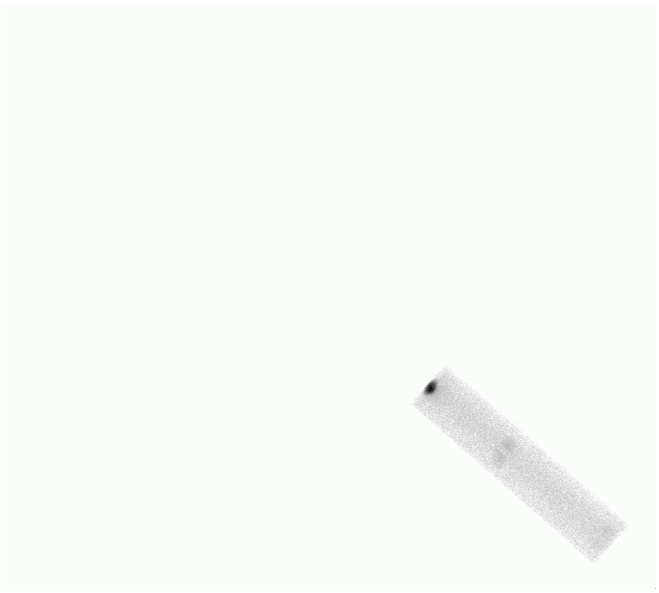

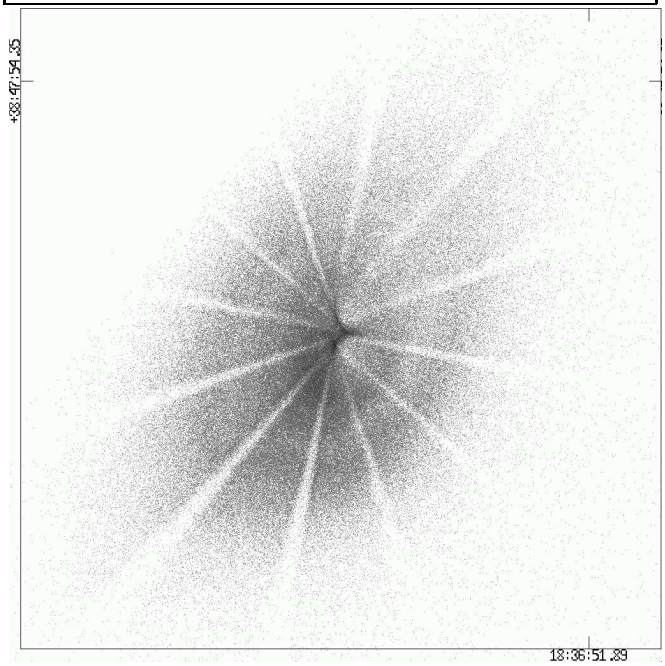

Chandra X-ray Center
Seq Num: 290326
Instrument: HRC
Obs ID: 5053
Source: Vega
PI: Dr. CXC Calibration
Title: AO5 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.2	Processing system revision
DATE	2006-06-04T10:36:52	Date and time of file creation
DATE-OBS	2004-02-05T03:46:30	Observation start date
DATE-END	2004-02-05T04:28:20	Observation end date
RA_PNT	279.5626323693	Pointing RA
DEC_PNT	39.005555848845	Pointing Dec
ROLL_PNT	41.04237082377	Pointing Roll
RA_TARG	279.235	Observer's specified target RA
DEC_TARG	38.783778	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.2	Processing system revision
DATE	2006-06-04T11:26:51	Date and time of file creation
DATE-OBS	2004-02-05T03:46:30	Observation start date
DATE-END	2004-02-05T04:28:20	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	NONE	Grating
OBJECT	Vega	Source name
TITLE	AO5 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5053	Observation id
SEQ_NUM	290326	Sequence number
RA_NOM	279.5626323693	Nominal RA
DEC_NOM	39.005555848845	Nominal Dec
ROLL_NOM	41.04237082377	Nominal Roll

Chandra X-ray Center
Seq Num: 290326
Instrument: HRC
Obs ID: 5053
Source: Vega
PI: Dr. CXC Calibration
Title: AO5 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

Full Field with Sources

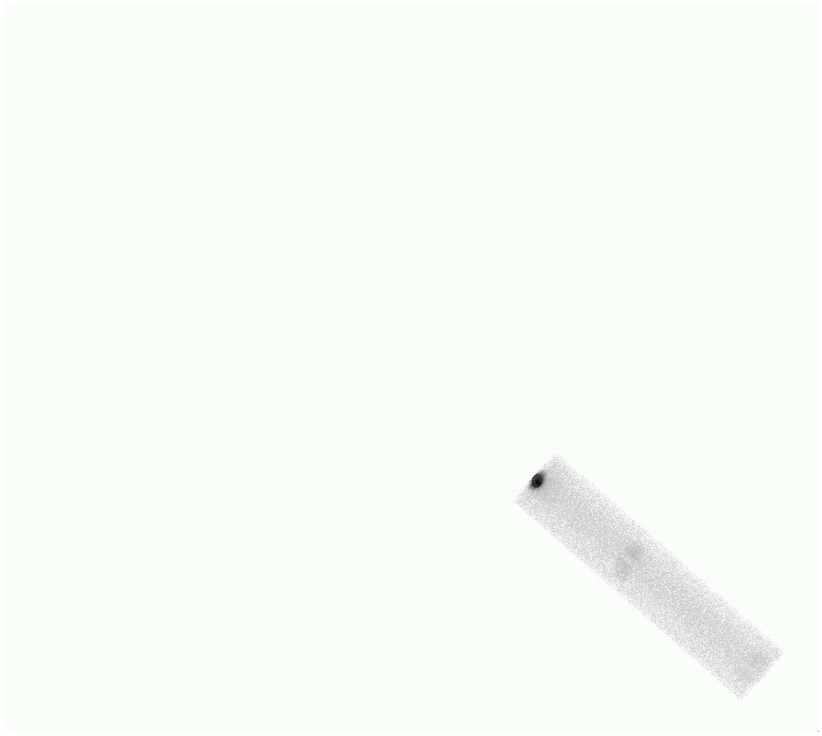

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
279.238343	38.782586	73219.023438	502.391754	145.740906