Chandra X-ray Center

Instrument: HRC
Source: HZ43
Grating: LETG
Title: AO6 Calibration Observations of HZ43

Seq Num: 290450
Obs ID: 5958
PI: Dr. CXC Calibration

hrcf05958N003 full img2.fits	hrcf05958N003 cntr img2.fits
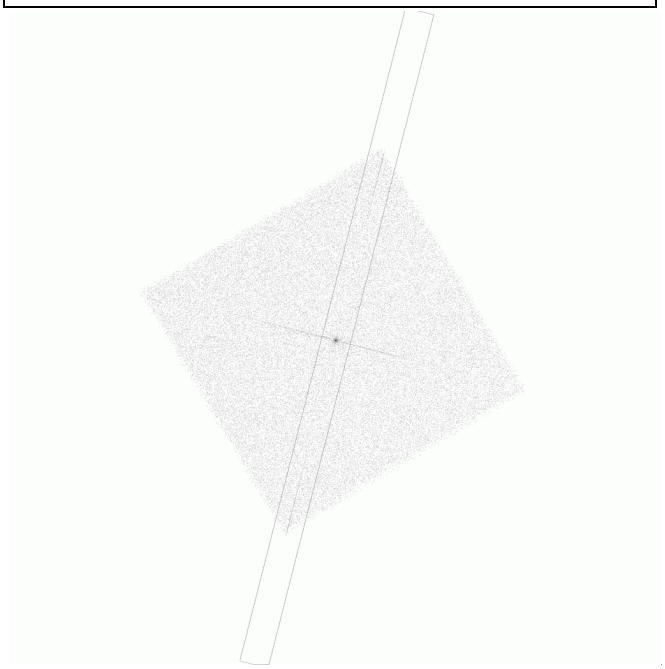	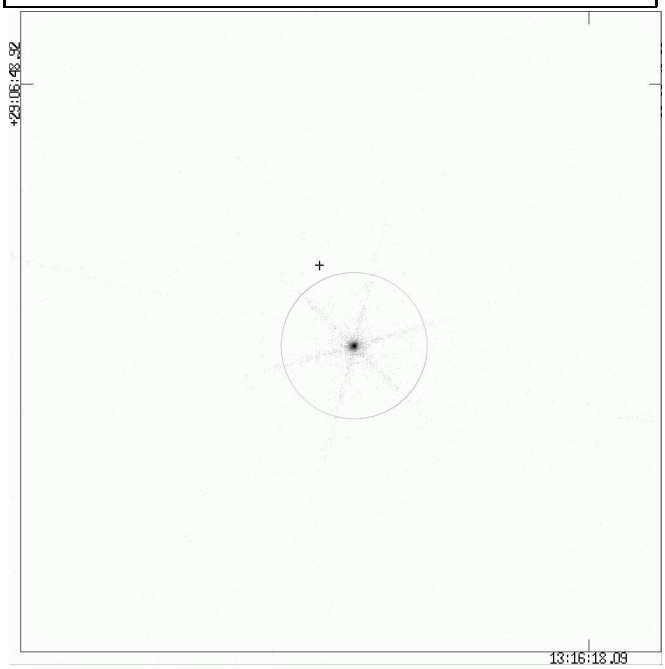

Chandra X-ray Center
Seq Num: 290450
Instrument: HRC
Obs ID: 5958
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO6 Calibration Observations of HZ43

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.2	ASCDS version number
DATE	2007-11-24T07:15:53	Date and time of file creation
DATE-OBS	2005-02-20T20:57:26	Observation start date
DATE-END	2005-02-20T21:56:35	Observation end date
RA_PNT	199.09305417438	Pointing RA
DEC_PNT	29.103182761386	Pointing Dec
ROLL_PNT	104.19046577436	Pointing Roll
RA_TARG	199.092083	Observer's specified target RA
DEC_TARG	29.099	Observer's specified target Dec
DEGAP	hrciD1999-07-22gaplookupN0003.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.11.2	ASCDS version number
DATE	2007-11-24T07:25:27	Date and time of file creation
DATE-OBS	2005-02-20T20:57:26	Observation start date
DATE-END	2005-02-20T21:56:35	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-I	Detector
GRATING	LETG	Grating
OBJECT	HZ43	Source name
TITLE	AO6 Calibration Observations of HZ43	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5958	Observation id
SEQ_NUM	290450	Sequence number
RA_NOM	199.09305417438	Nominal RA
DEC_NOM	29.103182761386	Nominal Dec
ROLL_NOM	104.19046577436	Nominal Roll

Chandra X-ray Center
Seq Num: 290450
Instrument: HRC
Obs ID: 5958
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO6 Calibration Observations of HZ43
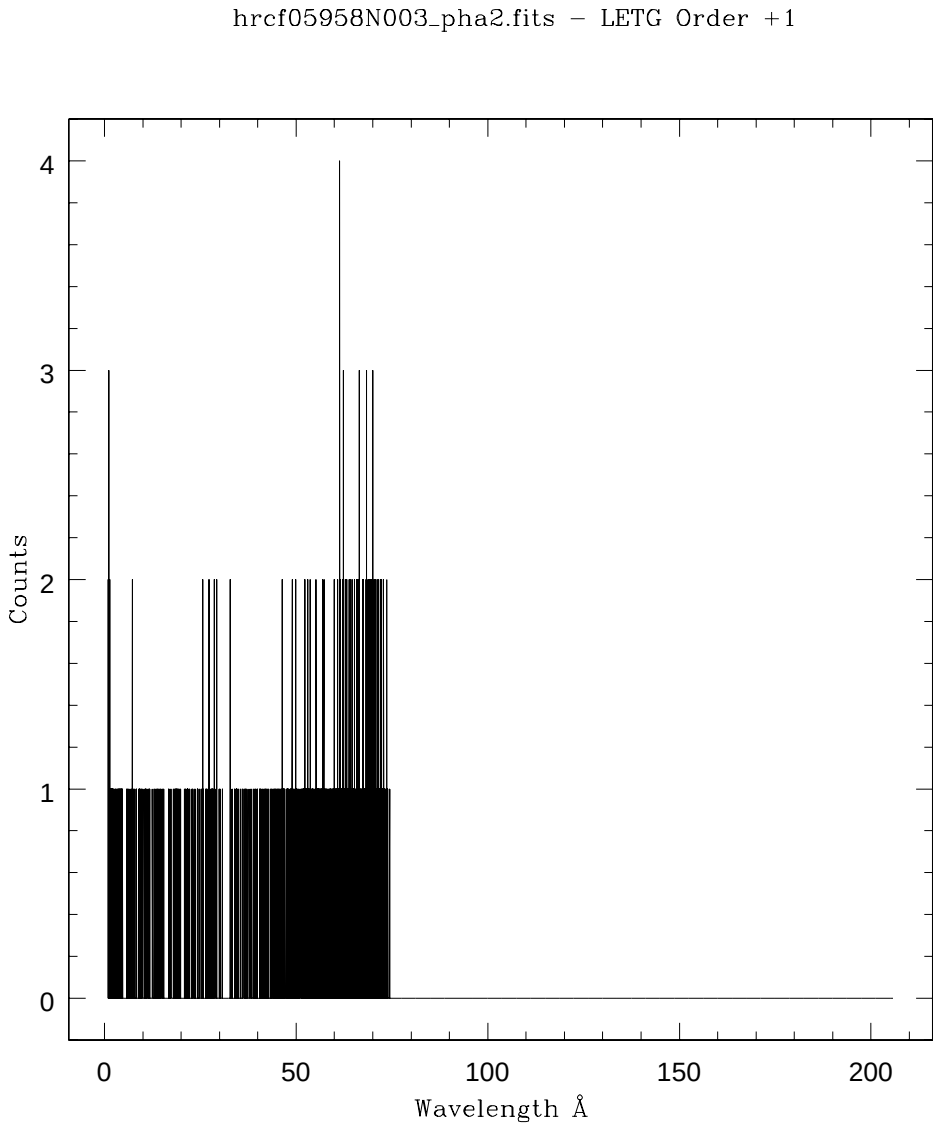
LETG +1 order