Chandra X-ray Center

Instrument: HRC
Source: HZ43
Grating: LETG
Title: AO6 Calibration Observations of HZ43

Seq Num: 290451
Obs ID: 5959
PI: Dr. CXC Calibration

hrcf05959N002 full img2.fits	hrcf05959N002 cntr img2.fits
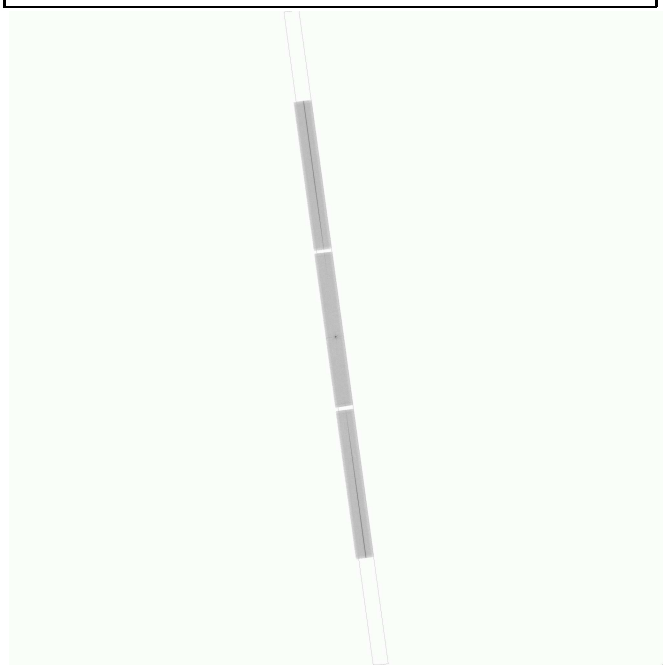	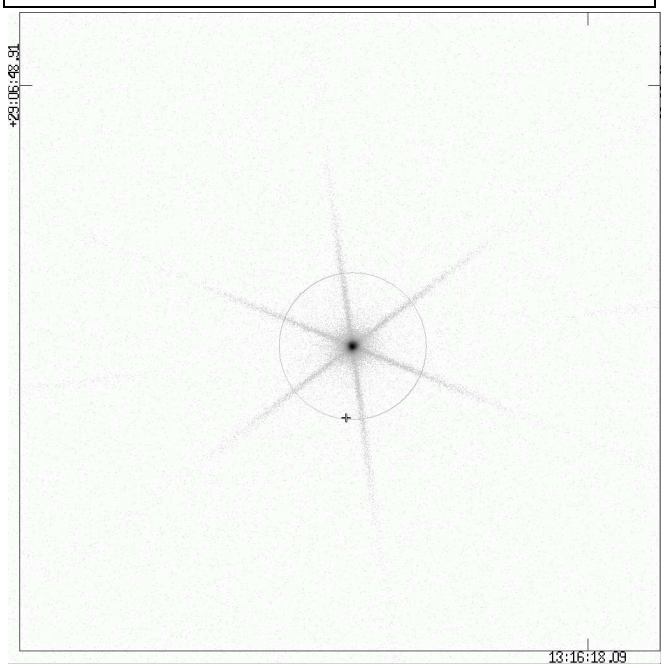

Chandra X-ray Center
Seq Num: 290451
Instrument: HRC
Obs ID: 5959
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO6 Calibration Observations of HZ43

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.1	ASCDS version number
DATE	2006-03-16T01:18:50	Date and time of file creation
DATE-OBS	2005-07-29T12:39:07	Observation start date
DATE-END	2005-07-29T18:03:35	Observation end date
RA_PNT	199.0912178105	Pointing RA
DEC_PNT	29.094446554325	Pointing Dec
ROLL_PNT	262.14359123673	Pointing Roll
RA_TARG	199.092083	Observer's specified target RA
DEC_TARG	29.099	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.1	ASCDS version number
DATE	2006-03-16T03:03:33	Date and time of file creation
DATE-OBS	2005-07-29T12:39:07	Observation start date
DATE-END	2005-07-29T18:03:35	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	LETG	Grating
OBJECT	HZ43	Source name
TITLE	AO6 Calibration Observations of HZ43	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5959	Observation id
SEQ_NUM	290451	Sequence number
RA_NOM	199.0912178105	Nominal RA
DEC_NOM	29.094446554325	Nominal Dec
ROLL_NOM	262.14359123673	Nominal Roll

Chandra X-ray Center
Seq Num: 290451
Instrument: HRC
Obs ID: 5959
Source: HZ43
PI: Dr. CXC Calibration
Grating: LETG
Title: AO6 Calibration Observations of HZ43
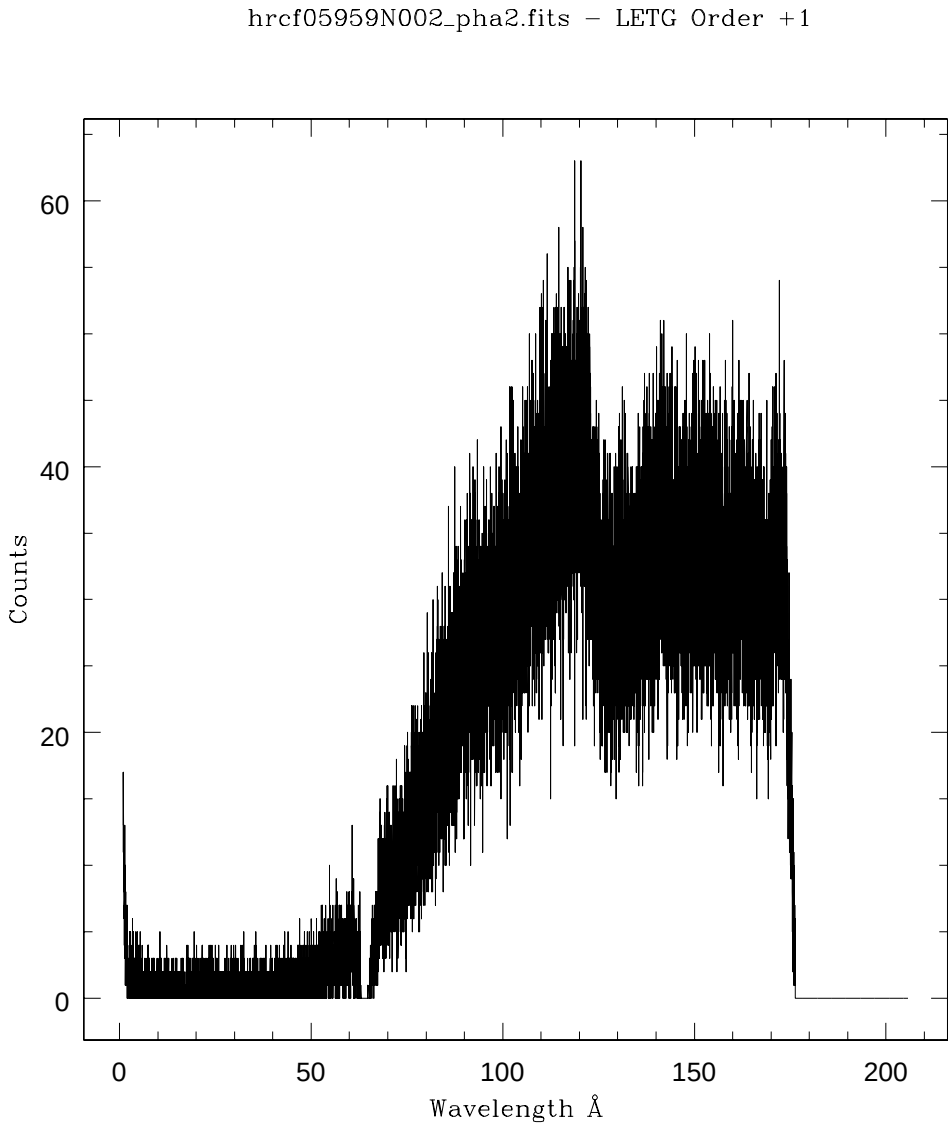
LETG +1 order