Chandra X-ray Center

Seq Num: 290460

Instrument: HRC

Obs ID: 5968

Source: Vega

PI: Dr. CXC Calibration

Title: AO6 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

---

hrcf05968N002 full img2.fits	hrcf05968N002 cntr img2.fits

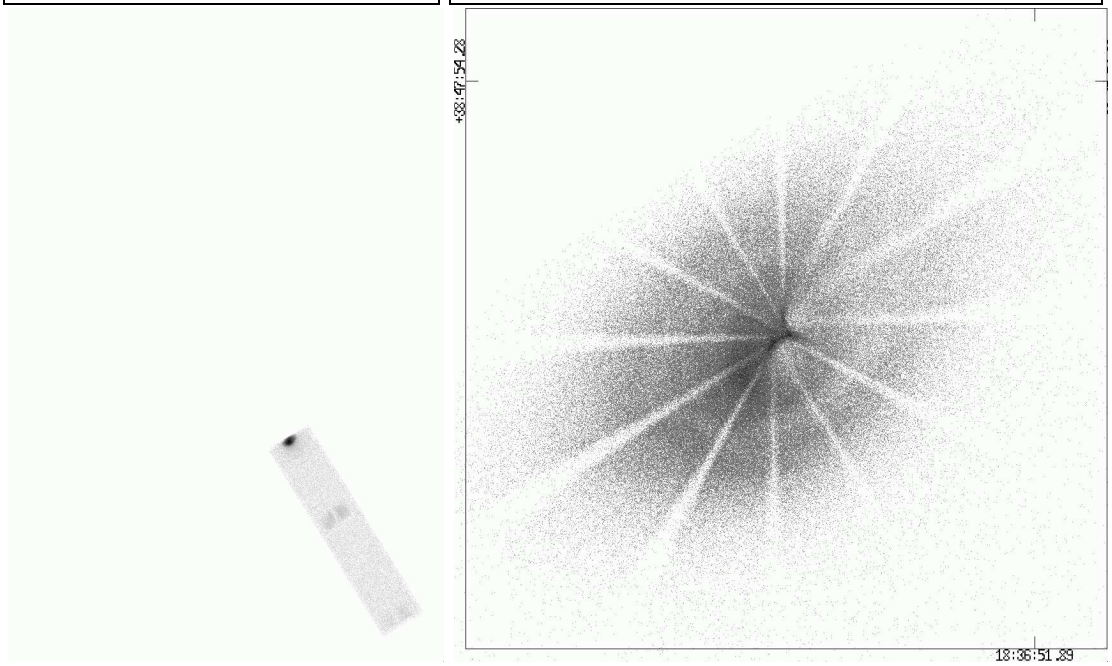

Chandra X-ray Center
Seq Num: 290460
Instrument: HRC
Obs ID: 5968
Source: Vega
PI: Dr. CXC Calibration
Title: AO6 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7	Processing system revision
DATE	2006-02-24T00:34:43	Date and time of file creation
DATE-OBS	2005-02-21T01:38:23	Observation start date
DATE-END	2005-02-21T02:20:13	Observation end date
RA_PNT	279.46346952462	Pointing RA
DEC_PNT	39.071293187142	Pointing Dec
ROLL_PNT	58.293173995124	Pointing Roll
RA_TARG	279.235	Observer's specified target RA
DEC_TARG	38.783778	Observer's specified target Dec
DEGAP	hrcsD1999-07-22gaplookupN0002.fits	

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7	Processing system revision
DATE	2006-02-24T01:03:43	Date and time of file creation
DATE-OBS	2005-02-21T01:38:23	Observation start date
DATE-END	2005-02-21T02:20:13	Observation end date
INSTRUME	HRC	Instrument
DETNAM	HRC-S	Detector
GRATING	NONE	Grating
OBJECT	Vega	Source name
TITLE	AO6 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	5968	Observation id
SEQ_NUM	290460	Sequence number
RA_NOM	279.46346952462	Nominal RA
DEC_NOM	39.071293187142	Nominal Dec
ROLL_NOM	58.293173995124	Nominal Roll

Chandra X-ray Center
Seq Num: 290460
Instrument: HRC
Obs ID: 5968
Source: Vega
PI: Dr. CXC Calibration
Title: AO6 Measurements of the optical/UV Transmission of the HRC and ACIS Filters.

Full Field with Sources

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
279.236924	38.783554	165735.656250	531.414001	311.876740