Chandra X-ray Center

Seq Num: 590376

Instrument: ACIS

Obs ID: 6049

Source: E0102-72[I3,-120,-7,0.5,0]

PI: Dr. CXC Calibration

Title: AO6A ACIS-I Calibration Observations of E0102-72

acisf06049N002 full img2.fits

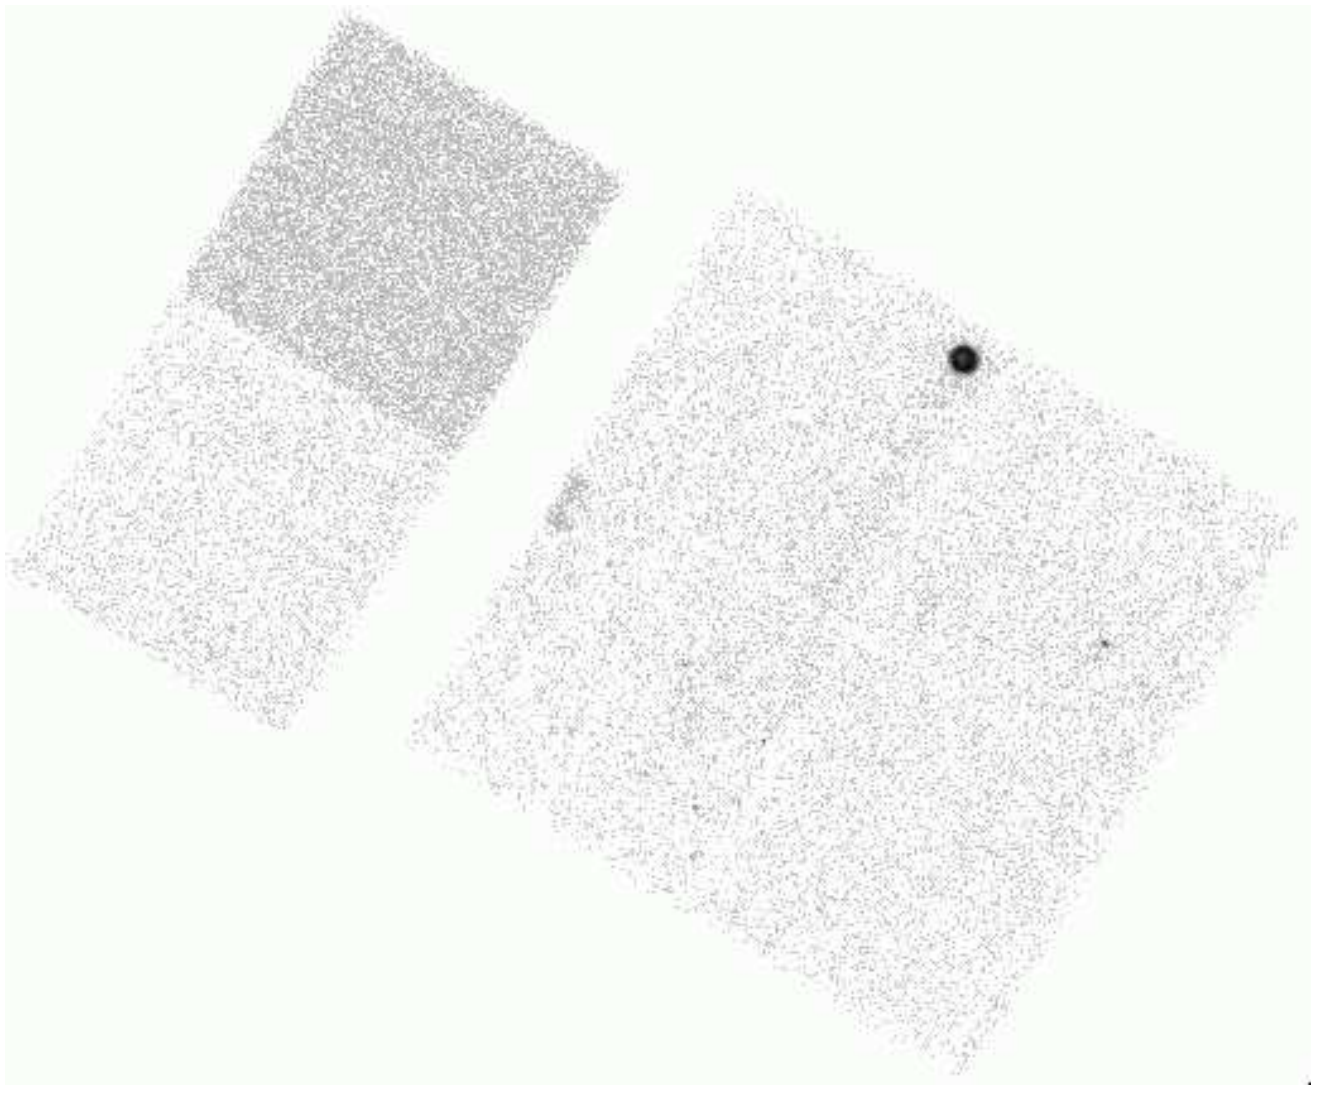

acisf06049N002 cntr img2.fits

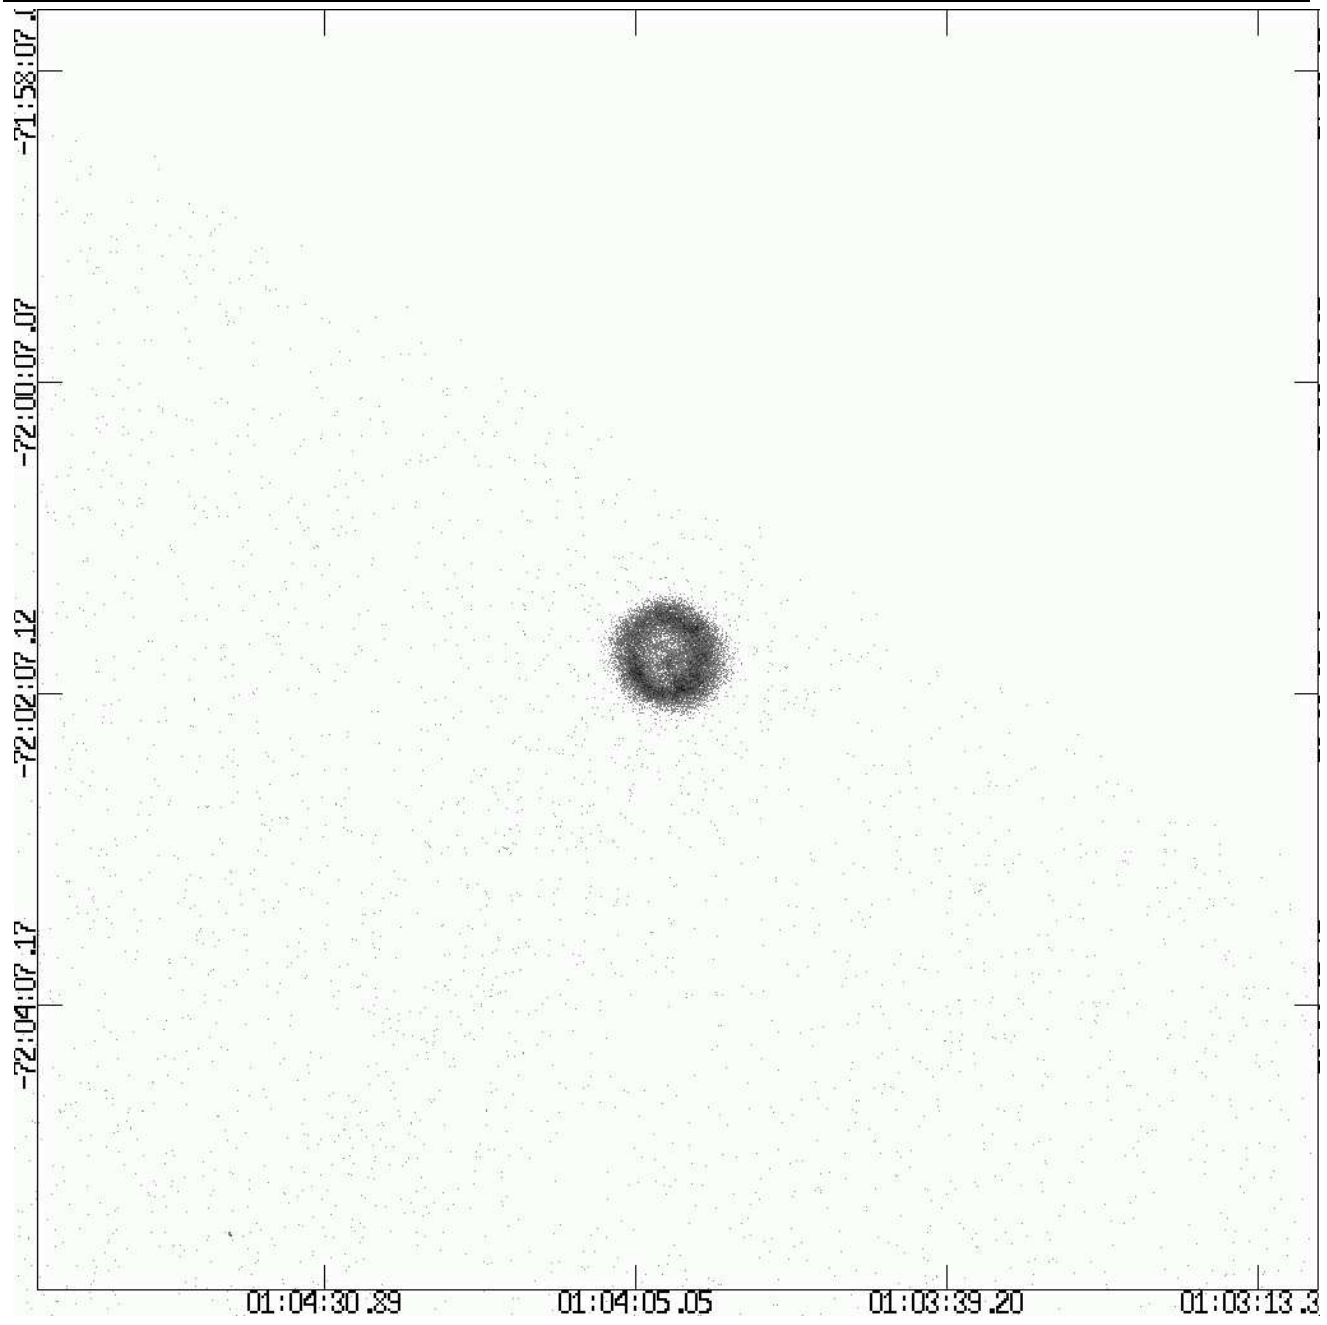

Chandra X-ray Center
Seq Num: 590376

Instrument: ACIS
Obs ID: 6049

Source: E0102-72[I3,-120,-7,0.5,0]
PI: Dr. CXC Calibration

Title: AO6A ACIS-I Calibration Observations of E0102-72

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.1	ASCDS version number
DATE	2006-04-08T19:30:20	Date and time of file creation
DATE-OBS	2004-12-13T01:12:36	Observation start date
DATE-END	2004-12-13T03:37:39	Observation end date
RA_PNT	16.184253392894	Pointing RA
DEC_PNT	-72.140815927764	Pointing Dec
ROLL_PNT	301.30541101312	Pointing Roll
RA_TARG	16.01	Observer's specified target RA
DEC_TARG	-72.032028	Observer's specified target Dec
DATAMODE	VFAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	153.76843262	Focal Plane Temperature [K]
FSW_VERS	31	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.1	ASCDS version number
DATE	2006-04-08T19:58:09	Date and time of file creation
DATE-OBS	2004-12-13T01:12:36	Observation start date
DATE-END	2004-12-13T03:37:39	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-012367	Detector
GRATING	NONE	Grating
OBJECT	E0102-72[I3,-120,-7,0.5,0]	Source name
TITLE	AO6A ACIS-I Calibration Observations of E0102-72	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	6049	Observation id
SEQ_NUM	590376	Sequence number
RA_NOM	16.184253392894	Nominal RA
DEC_NOM	-72.140815927764	Nominal Dec
ROLL_NOM	301.30541101312	Nominal Roll

Chandra X-ray Center

Seq Num: 590376

Instrument: ACIS

Obs ID: 6049

Source: E0102-72[I3,-120,-7,0.5,0]

PI: Dr. CXC Calibration

Title: AO6A ACIS-I Calibration Observations of E0102-72

Full Field with Sources

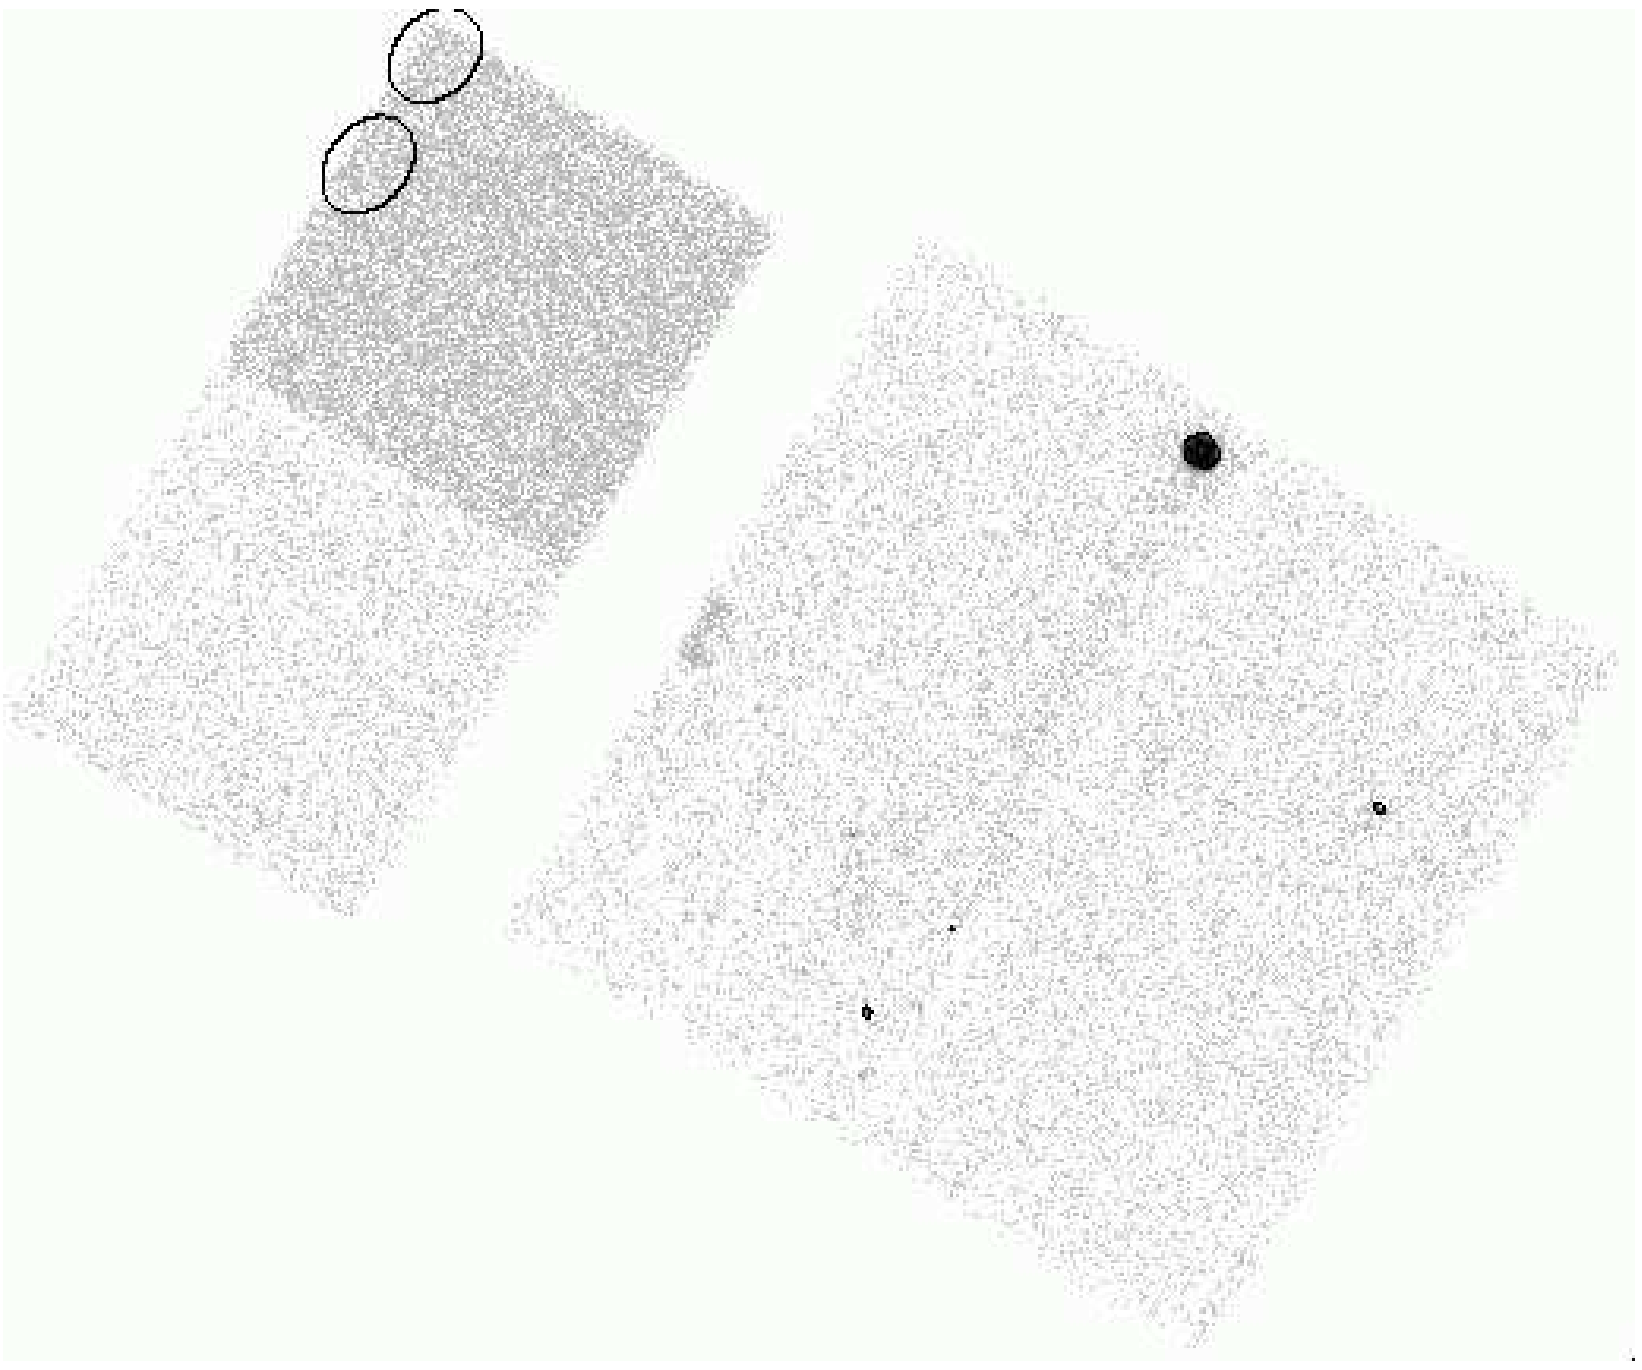

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
16.003453	-72.034526	1176.993164	67.226646	17.507835
16.004552	-72.027644	1138.102295	65.879799	17.275436
16.020251	-72.032589	1017.579285	60.397980	16.847902
16.019828	-72.028810	806.284119	57.254520	14.082453
15.997643	-72.032447	791.806824	69.588547	11.378407
15.807985	-72.153921	165.103455	15.263898	10.816598
16.290301	-72.196360	79.477272	10.781405	7.371698
16.864700	-71.892841	117.146278	22.676254	5.166033
16.387467	-72.225184	43.692501	8.547021	5.112015
16.941095	-71.930491	93.863785	24.020645	3.907630