Chandra X-ray Center

Seq Num: 590377

Instrument: ACIS

Obs ID: 6050

Source: E0102-72[I3,-120,-4,0.5,0]

PI: Dr. CXC Calibration

Title: AO6A ACIS-I Calibration Observations of E0102-72

---

acisf06050N002 full img2.fits

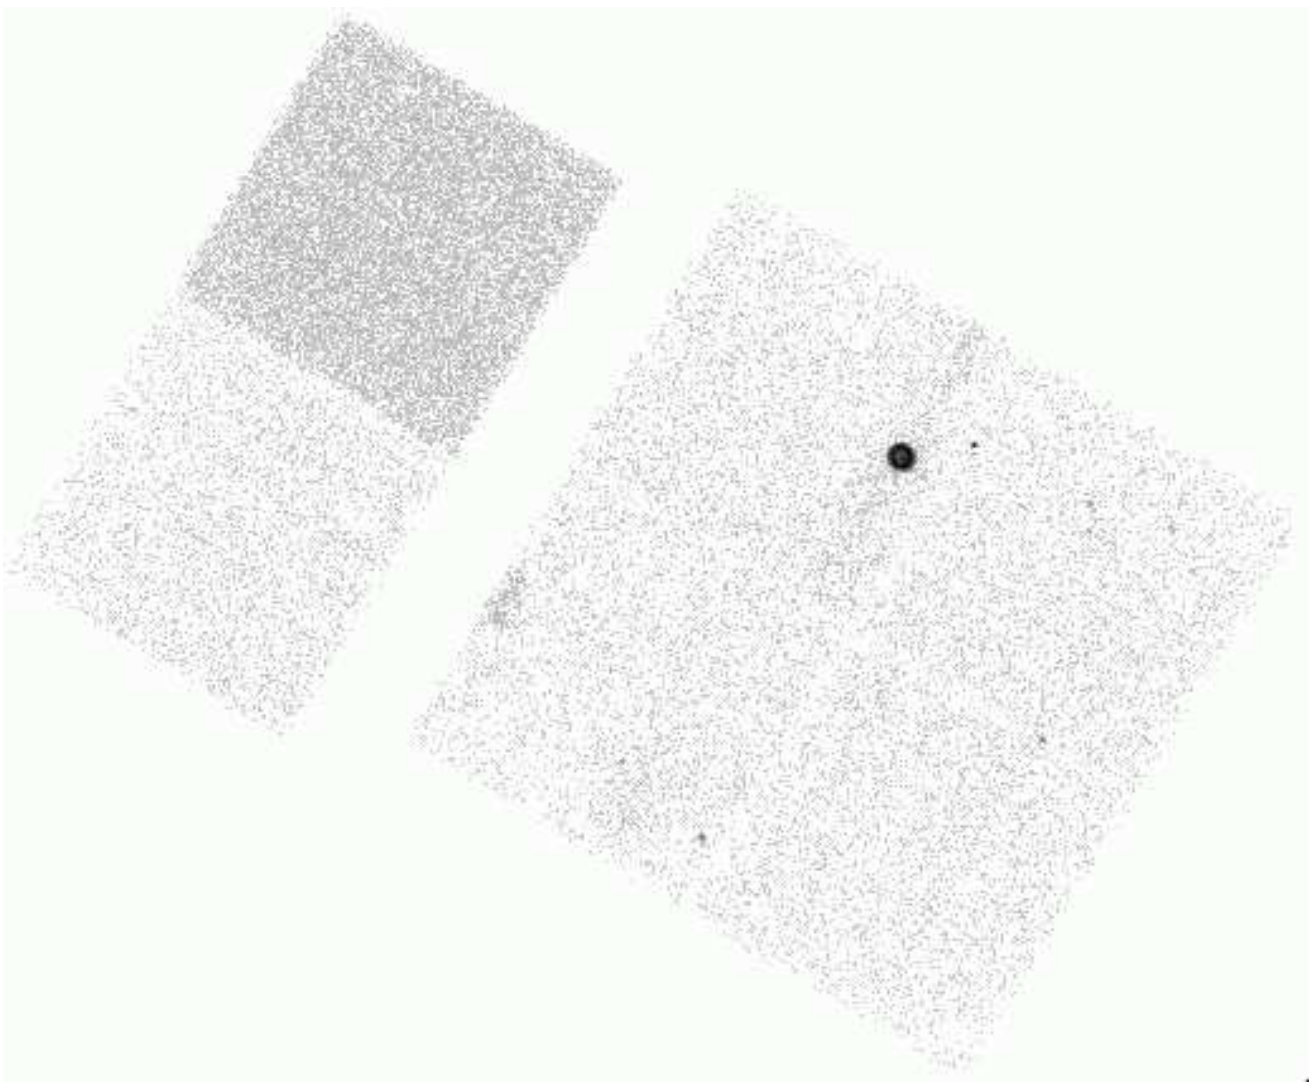

acisf06050N002 cntr img2.fits

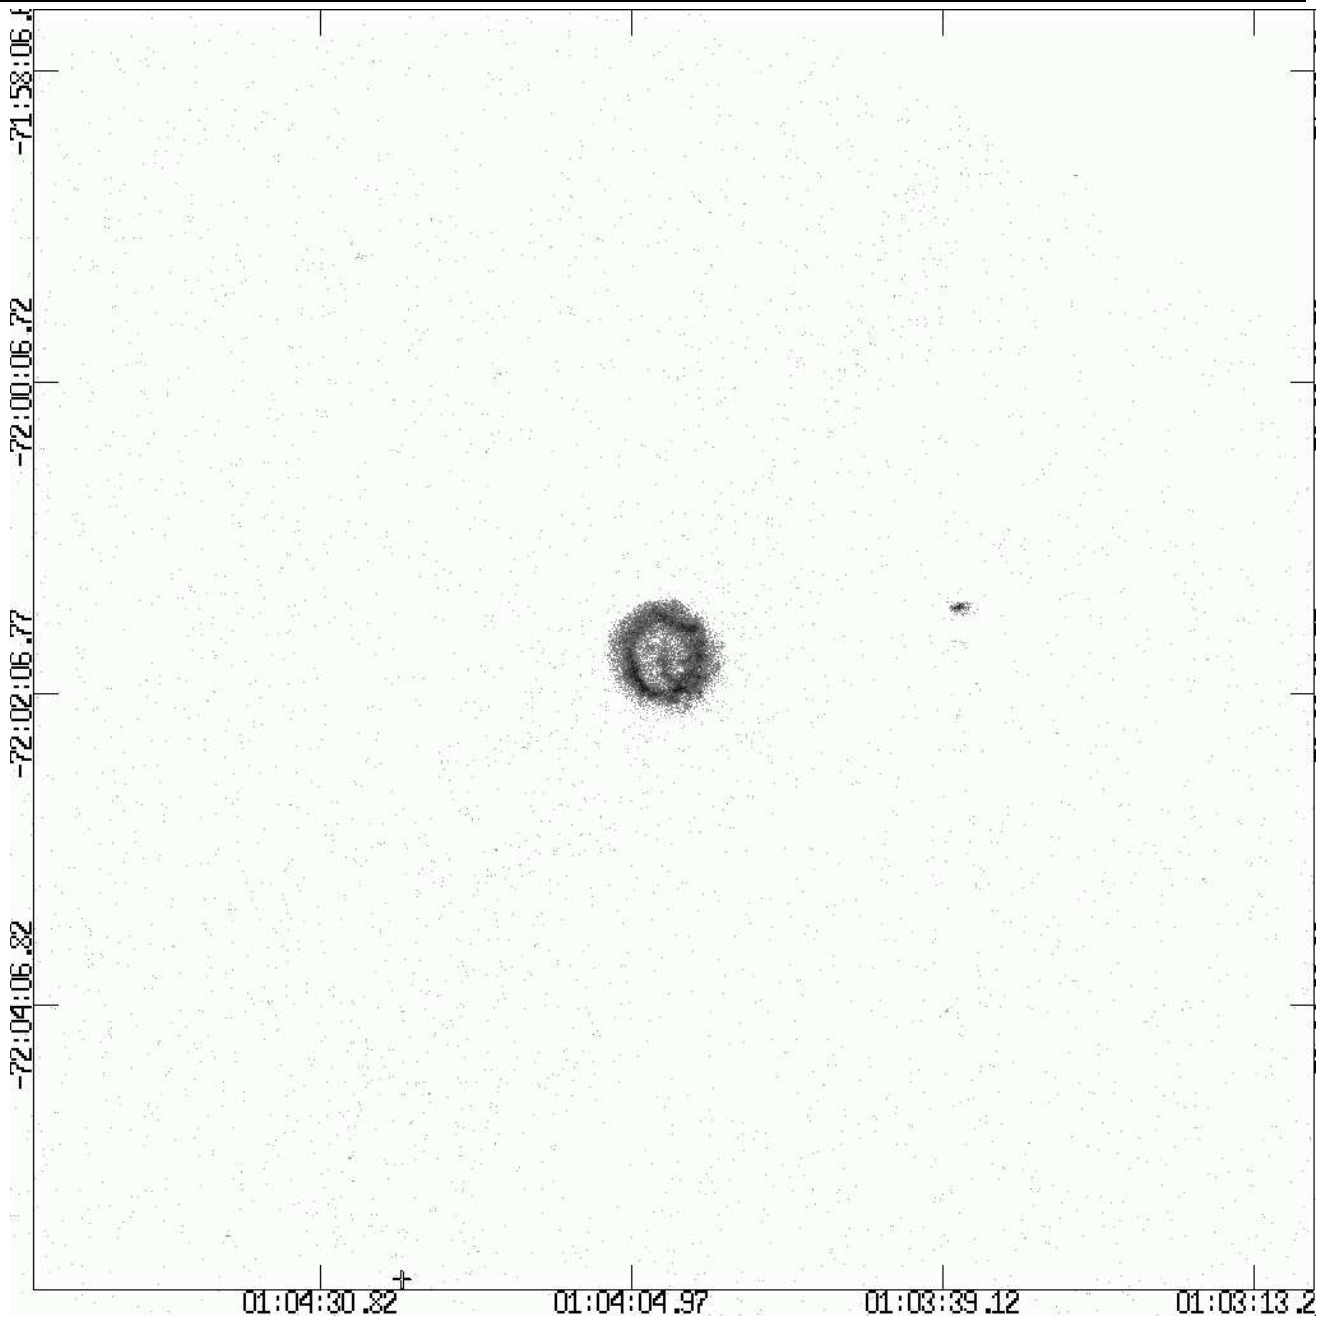

Chandra X-ray Center
Seq Num: 590377

Instrument: ACIS
Obs ID: 6050

Source: E0102-72[I3,-120,-4,0.5,0]
PI: Dr. CXC Calibration

Title: AO6A ACIS-I Calibration Observations of E0102-72

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.1	ASCDS version number
DATE	2006-04-08T19:43:06	Date and time of file creation
DATE-OBS	2004-12-13T03:37:39	Observation start date
DATE-END	2004-12-13T06:02:53	Observation end date
RA_PNT	16.099963262871	Pointing RA
DEC_PNT	-72.098026253166	Pointing Dec
ROLL_PNT	301.13203320344	Pointing Roll
RA_TARG	16.01	Observer's specified target RA
DEC_TARG	-72.032028	Observer's specified target Dec
DATAMODE	VFAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	154.09092712	Focal Plane Temperature [K]
FSW_VERS	31	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.7.1	ASCDS version number
DATE	2006-04-08T20:22:35	Date and time of file creation
DATE-OBS	2004-12-13T03:37:39	Observation start date
DATE-END	2004-12-13T06:02:53	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-012367	Detector
GRATING	NONE	Grating
OBJECT	E0102-72[I3,-120,-4,0.5,0]	Source name
TITLE	AO6A ACIS-I Calibration Observations of E0102-72	Proposal title
OBSERVER	Dr. CXC Calibration	Principal investigator
OBS_ID	6050	Observation id
SEQ_NUM	590377	Sequence number
RA_NOM	16.099963262871	Nominal RA
DEC_NOM	-72.098026253166	Nominal Dec
ROLL_NOM	301.13203320344	Nominal Roll

Chandra X-ray Center

Seq Num: 590377

Instrument: ACIS

Obs ID: 6050

Source: E0102-72[I3,-120,-4,0.5,0]

PI: Dr. CXC Calibration

Title: AO6A ACIS-I Calibration Observations of E0102-72

Full Field with Sources

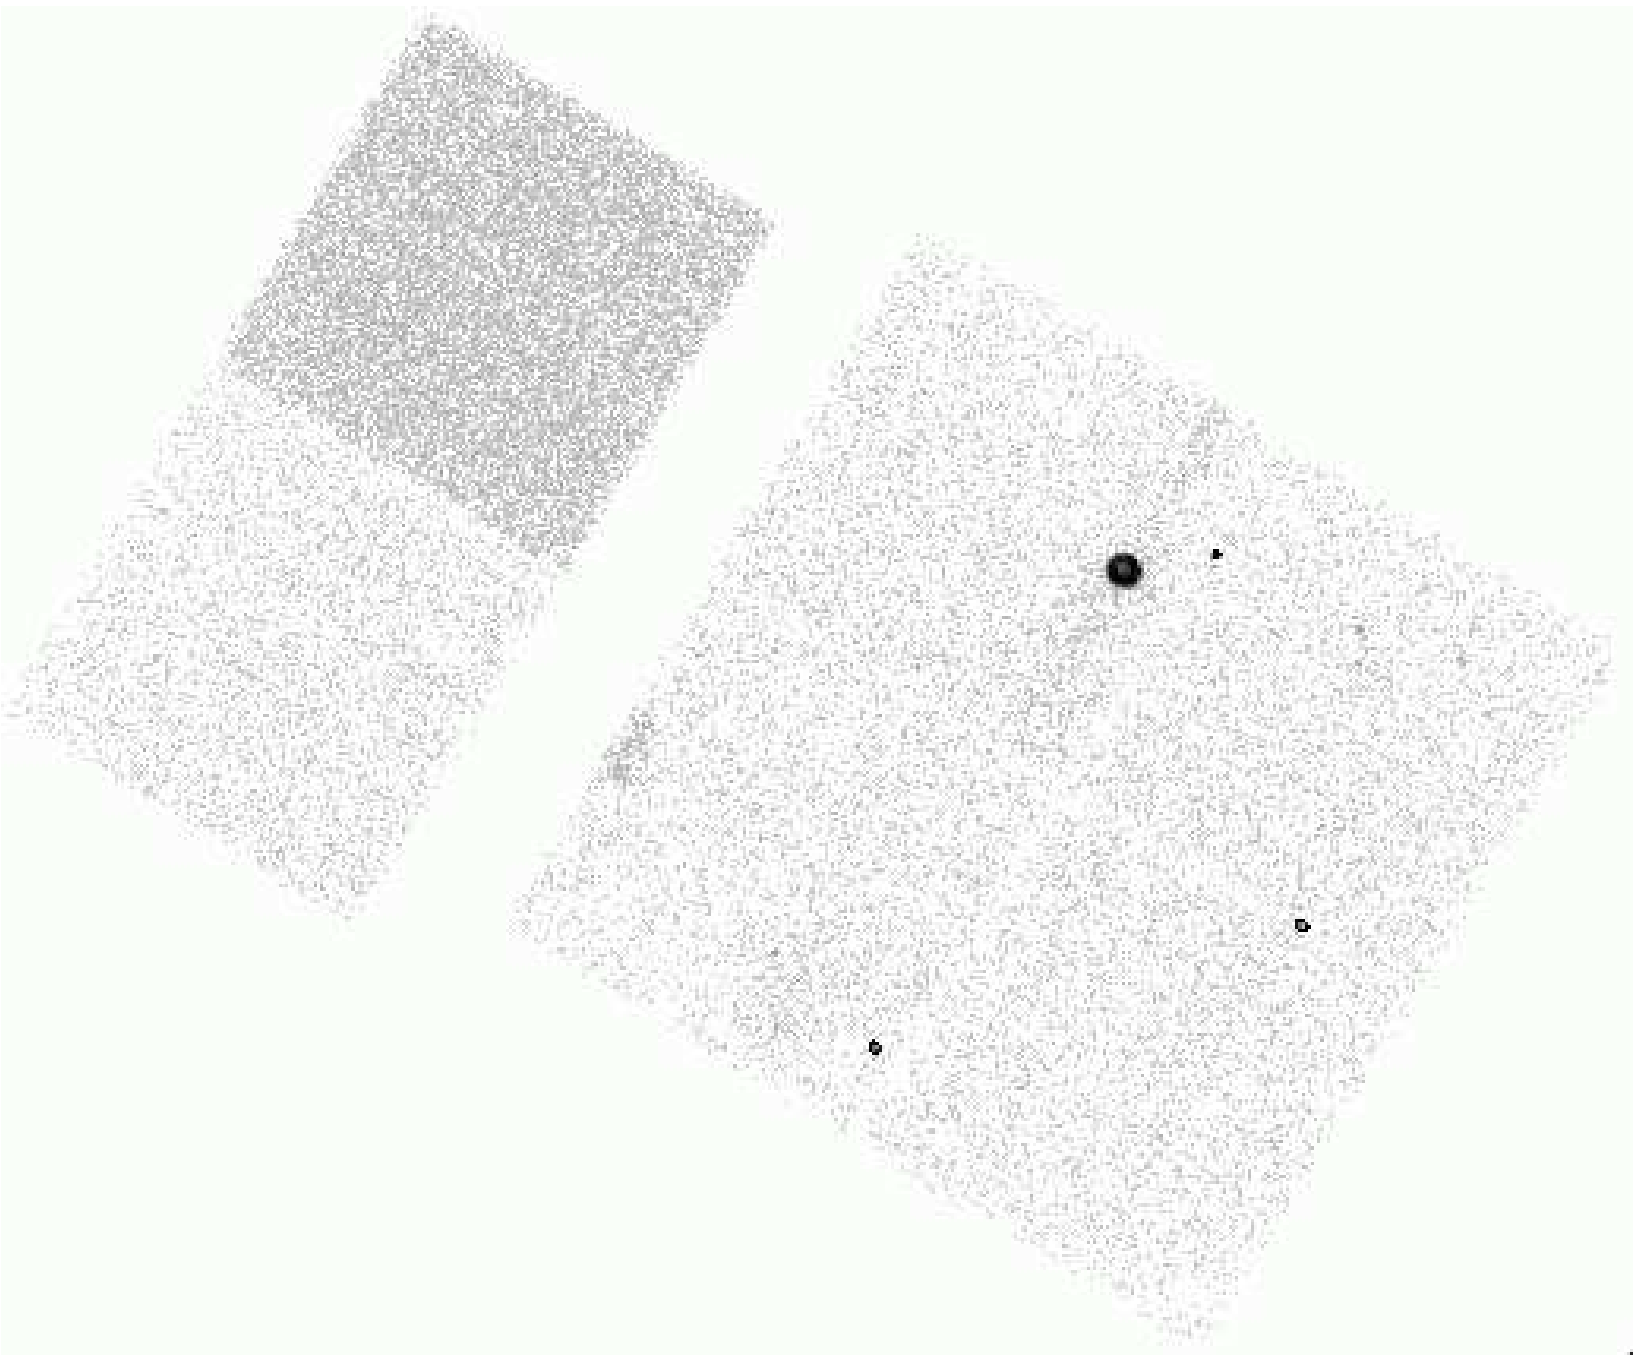

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
15.906188	-72.025909	331.795441	19.880486	16.689505
16.014915	-72.034973	434.428558	42.792156	10.152061
16.019755	-72.032969	459.000000	47.500965	9.662962
16.002723	-72.034590	461.714294	49.537018	9.320591
15.999212	-72.028165	402.714294	43.370689	9.285401
16.011530	-72.035184	312.714294	39.669319	7.883027
16.290590	-72.196360	76.062073	11.046794	6.885443
16.020368	-72.031386	264.428558	40.423428	6.541469
15.995934	-72.031285	270.285706	41.432869	6.523461
15.807642	-72.153912	63.692501	9.782299	6.510995