Chandra X-ray Center

Seq Num: 400306

Instrument: ACIS

Obs ID: 3819

Source: A1118-616

PI: PROF. LARS BILDSTEN

Title: QUIESCENT EMISSION FROM TRANSIENT ACCRETION-POWERED PULSARS

---

acisf03819N002 full img2.fits

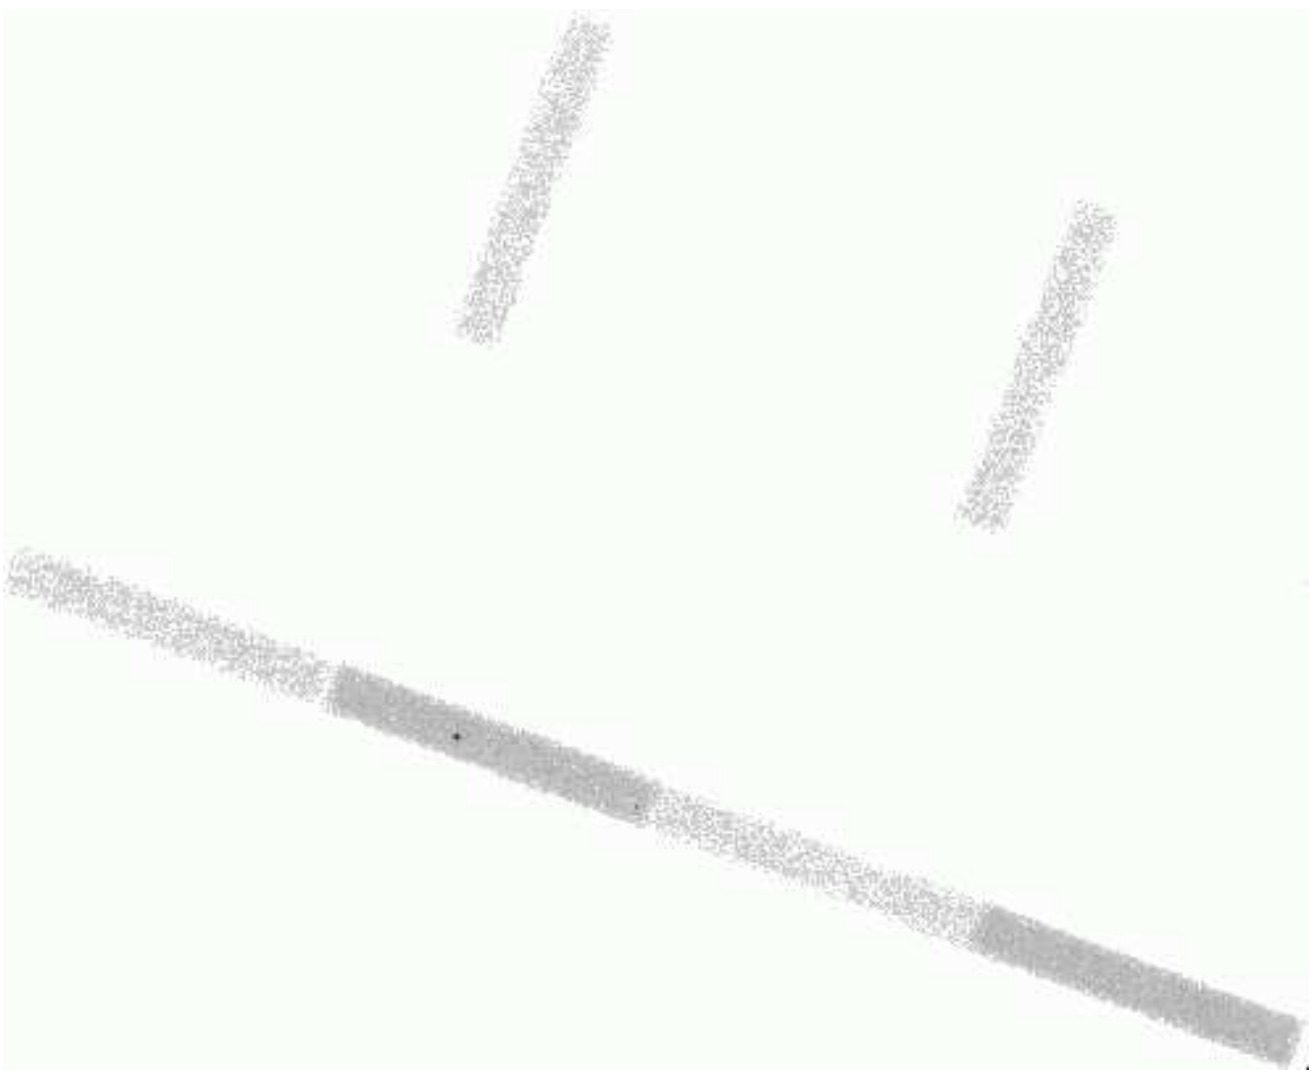

acisf03819N002 cntr img2.fits

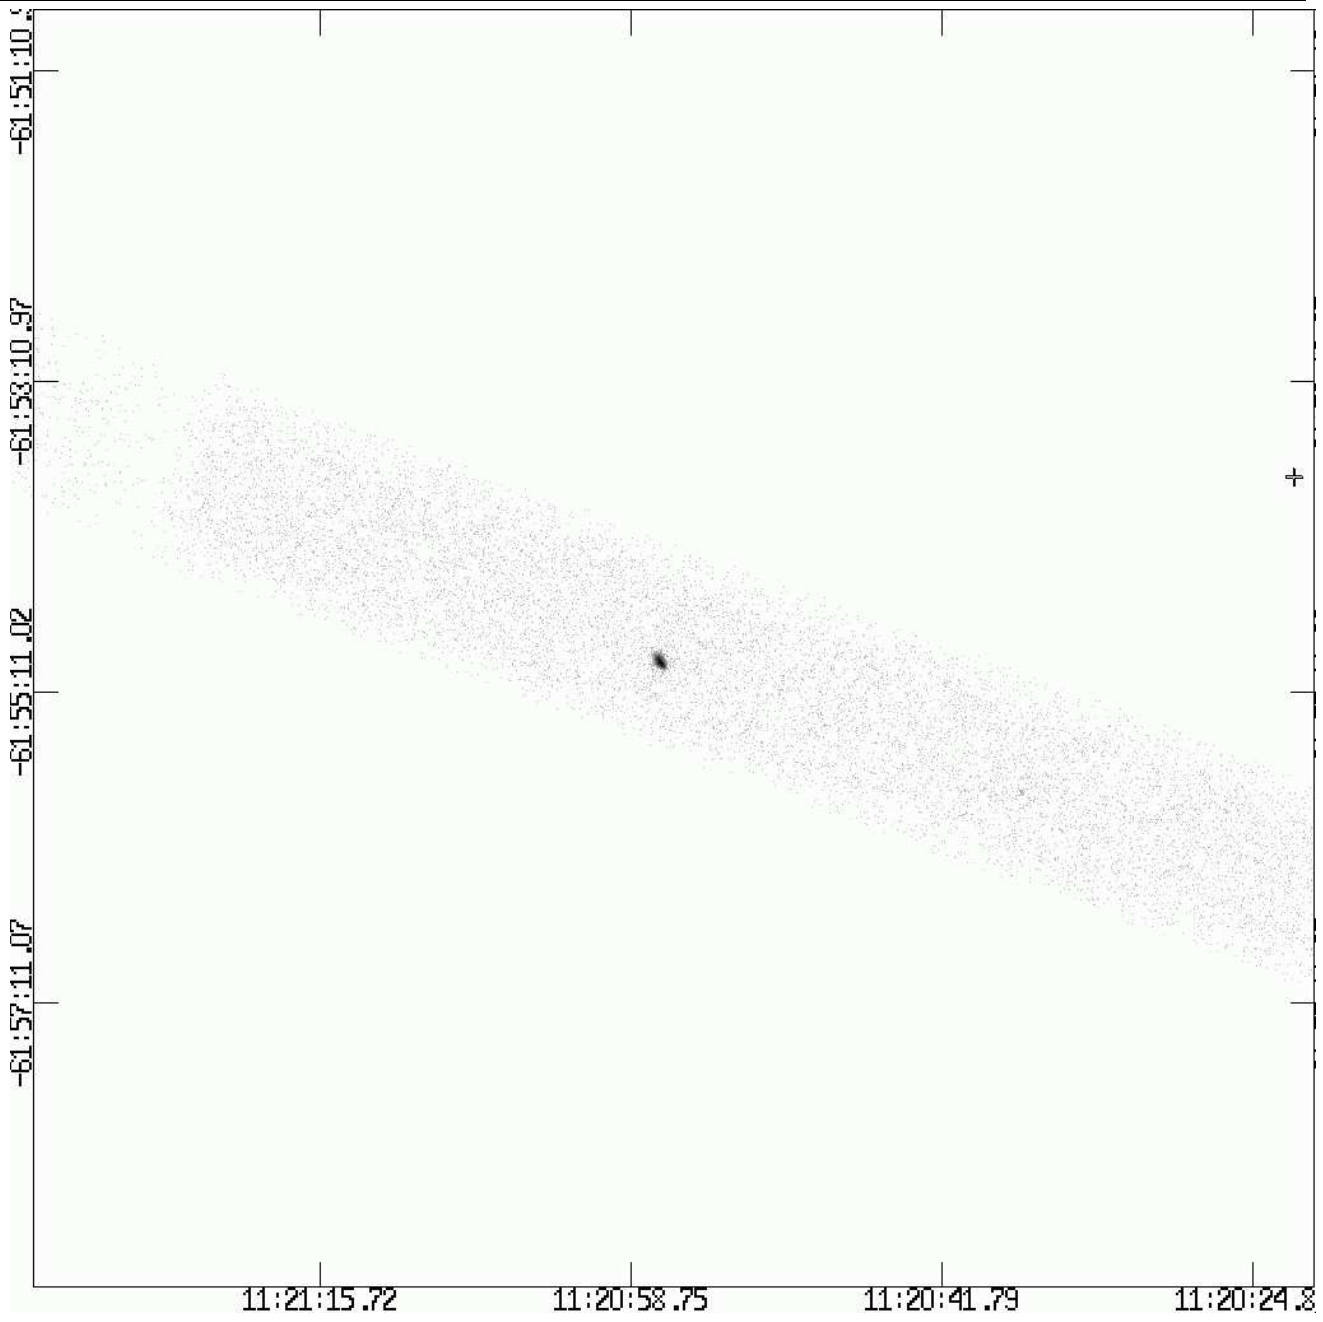

Chandra X-ray Center Seq Num: 400306

Instrument: ACIS Obs ID: 3819

Source: A1118-616 PI: PROF. LARS BILDSTEN

Title: QUIESCENT EMISSION FROM TRANSIENT ACCRETION-POWERED PULSARS

Level 1 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-07-07T13:19:37	Date and time of file creation
DATE-OBS	2003-08-21T07:58:56	Observation start date
DATE-END	2003-08-21T14:04:59	Observation end date
RA_PNT	170.09393158401	Pointing RA
DEC_PNT	-61.897002694991	Pointing Dec
ROLL_PNT	200.46347413323	Pointing Roll
RA_TARG	170.238333	Observer's specified target RA
DEC_TARG	-61.91675	Observer's specified target Dec
DATAMODE	FAINT	Data mode
READMODE	TIMED	Read mode
FP_TEMP	153.4460144	Focal Plane Temperature [K]
FSW_VERS	30	ACIS flight software version number

Level 2 Observational Parameters		
Parameter	Value	Description
ASCDSVER	7.6.8	ASCDS version number
DATE	2006-07-07T13:56:16	Date and time of file creation
DATE-OBS	2003-08-21T07:58:56	Observation start date
DATE-END	2003-08-21T14:04:59	Observation end date
INSTRUME	ACIS	Instrument
DETNAM	ACIS-235678	Detector
GRATING	NONE	Grating
OBJECT	A1118-616	Source name
TITLE	QUIESCENT EMISSION FROM TRAN- SIENT ACCRETION-POWERED PULSARS	Propos
OBSERVER	PROF. LARS BILDSTEN	Principal investigator
OBS_ID	3819	Observation id
SEQ_NUM	400306	Sequence number
RA_NOM	170.09393158401	Nominal RA
DEC_NOM	-61.897002694991	Nominal Dec
ROLL_NOM	200.46347413323	Nominal Roll

Chandra X-ray Center

Seq Num: 400306

Instrument: ACIS

Obs ID: 3819

Source: A1118-616

PI: PROF. LARS BILDSTEN

Title: QUIESCENT EMISSION FROM TRANSIENT ACCRETION-POWERED PULSARS

Full Field with Sources

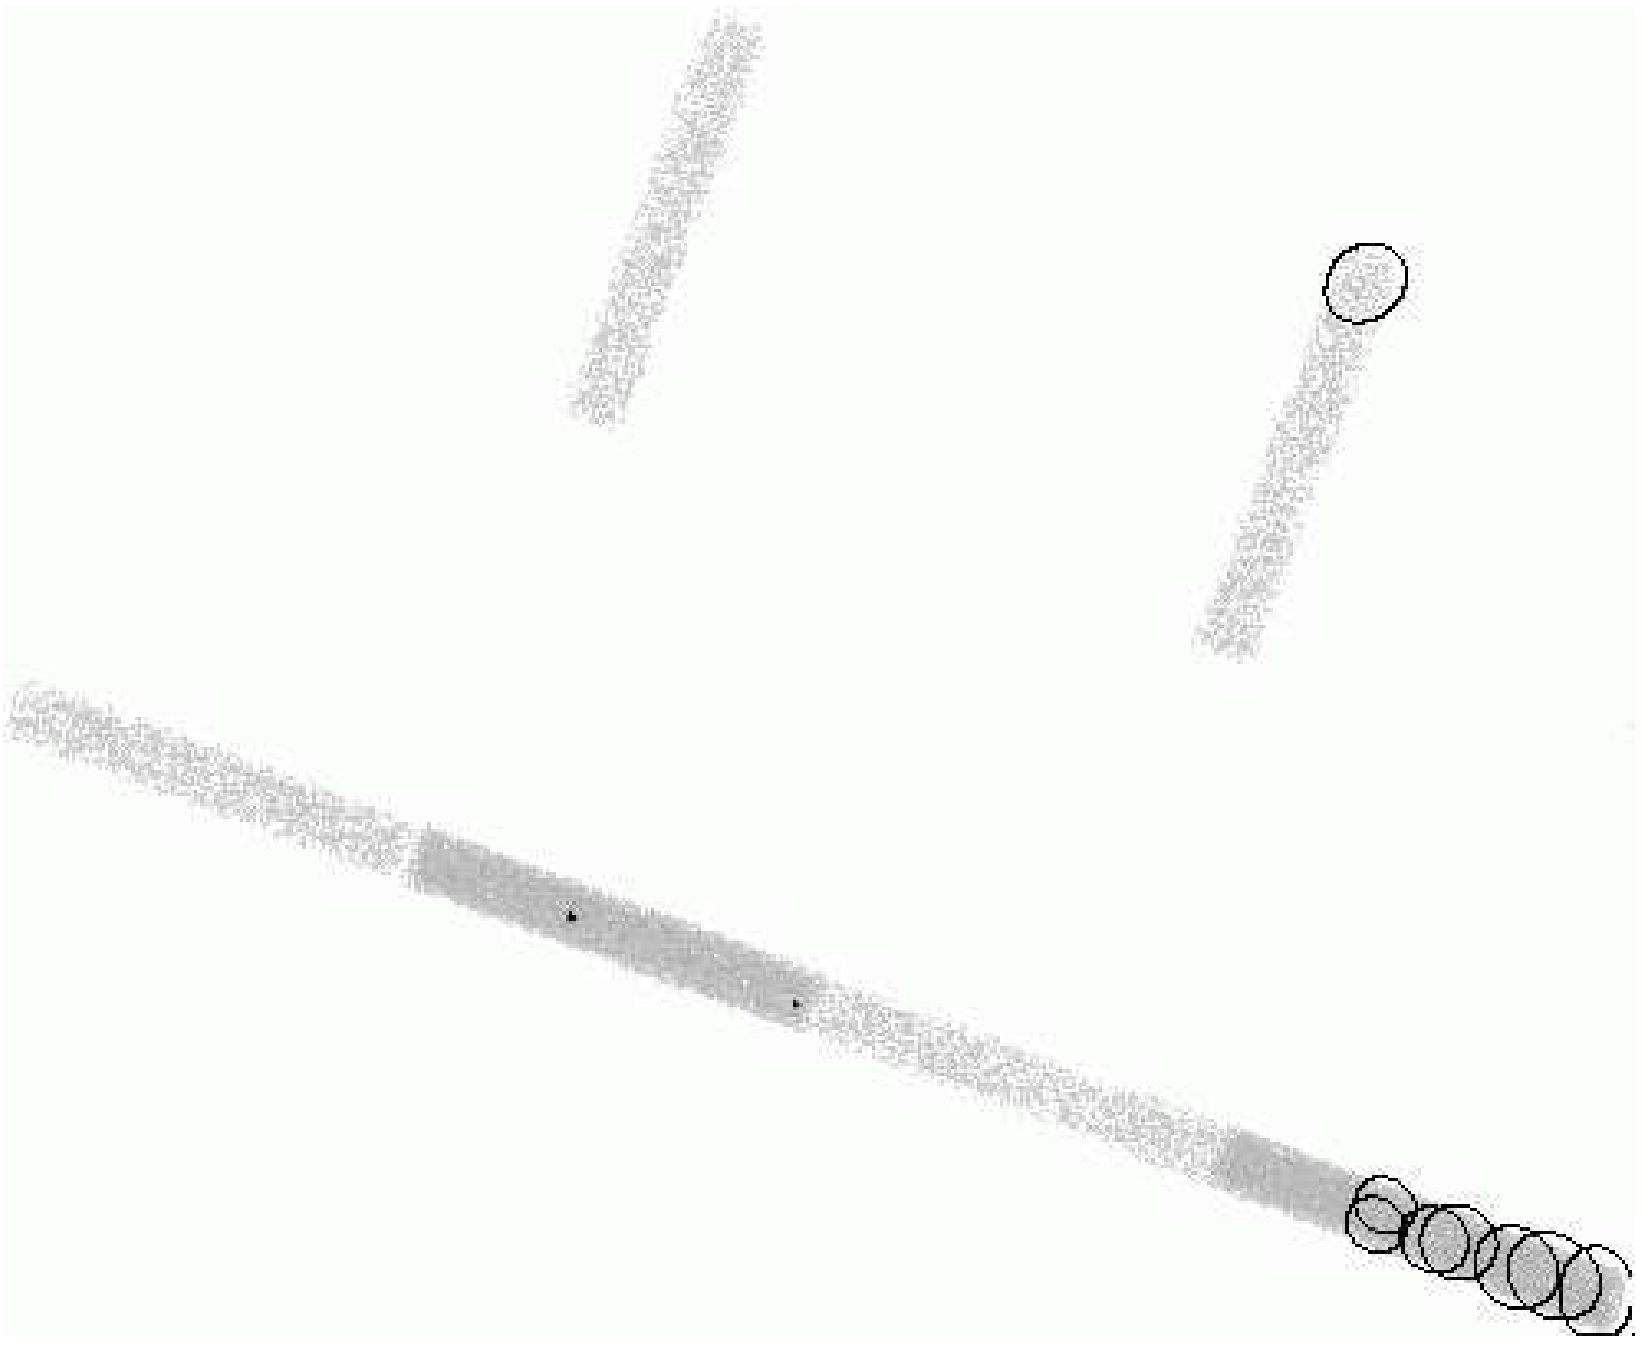

List of the Brighest Sources in the Field				
RA[deg]	DEC[deg]	NET_COUNTS[count]	NET_COUNTS_ERR[count]	SNR
170.238207	-61.916710	3832.000000	65.945442	58.108639
169.512551	-62.040304	711.156128	43.046654	16.520590
169.542964	-62.034800	591.875916	50.938606	11.619397
169.569081	-62.032095	582.750000	50.772938	11.477571
169.610427	-62.023913	418.500000	44.916527	9.317284
169.680562	-61.705473	122.833336	18.319502	6.705059
169.668956	-62.018190	211.235291	34.377110	6.144650
170.080007	-61.945855	89.714287	14.839802	6.045518
169.662795	-62.011656	171.862747	35.670273	4.818094
169.627414	-62.023122	193.655167	40.537472	4.777189